

Sample Name :β-Amyloid (4-10)
 Cat No. :RP20173
 Lot No. :E4830719I
 Time Processed :3:40:22 PM
 Month-Day-Year Processed :09/23/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

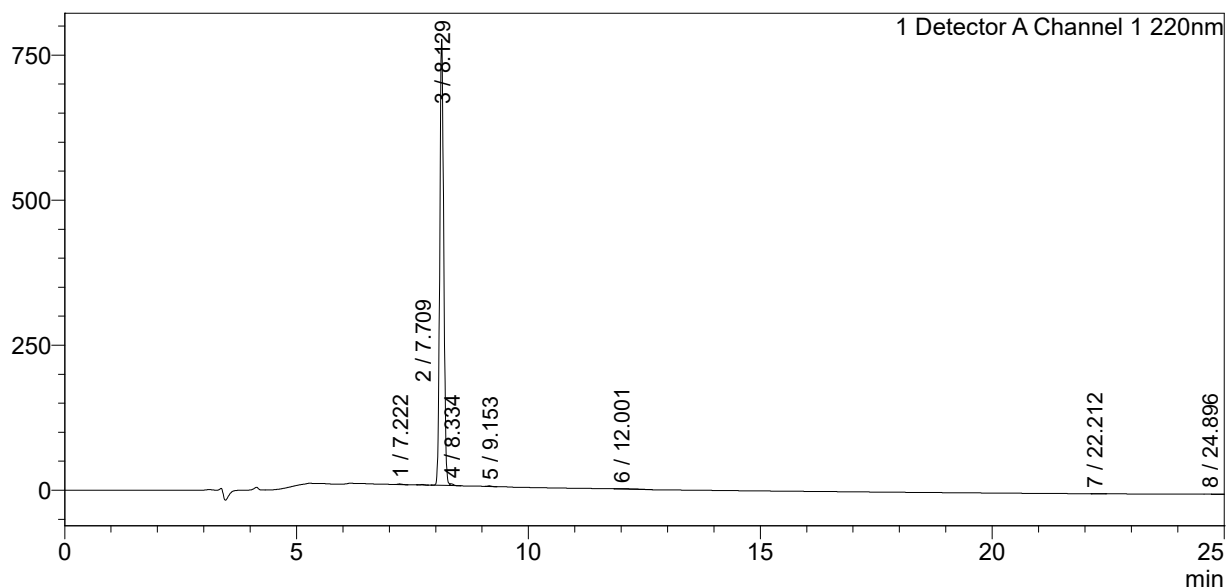

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.222	5744	964	0.125
2	7.709	5677	1003	0.123
3	8.129	4545502	769409	98.766
4	8.334	14463	3055	0.314
5	9.153	6654	1149	0.145
6	12.001	20771	555	0.451
7	22.212	1376	133	0.030
8	24.896	2086	229	0.045
Total		4602273	776496	100.000