

Sample Name :Orphanin FQ/Nociceptin, human, mouse, ox, rat
 Cat No. : RP13084
 Lot No. : E4882019I
 Time Processed :9:58:52 AM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

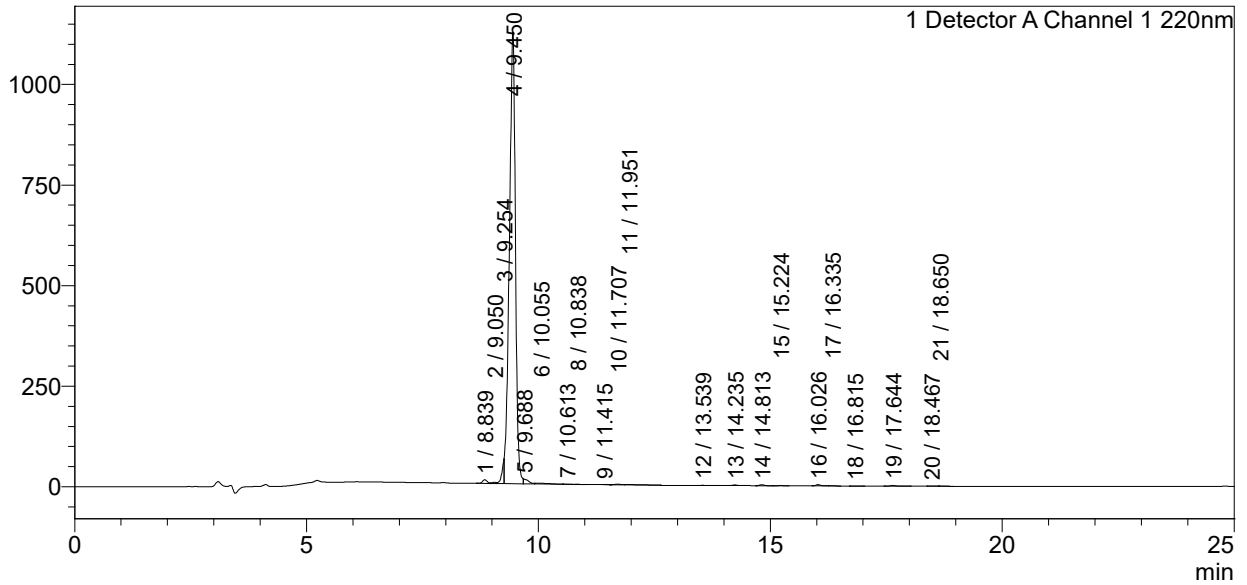

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.839	65977	9225	0.611
2	9.050	19725	2910	0.183
3	9.254	198772	55465	1.840
4	9.450	10272616	1122836	95.069
5	9.688	89654	11902	0.830
6	10.055	39900	2092	0.369
7	10.613	1768	224	0.016
8	10.838	2124	365	0.020
9	11.415	1303	212	0.012
10	11.707	13995	1448	0.130
11	11.951	20811	694	0.193
12	13.539	4293	547	0.040
13	14.235	11873	1589	0.110
14	14.813	17681	2473	0.164
15	15.224	4450	525	0.041

Peak#	Ret. Time	Area	Height	Area%
16	16.026	20748	3178	0.192
17	16.335	1429	201	0.013
18	16.815	1313	163	0.012
19	17.644	13755	1519	0.127
20	18.467	1718	138	0.016
21	18.650	1522	122	0.014
Total		10805429	1217830	100.000