

Sample Name :Kemptide  
 Cat No. :RP10287  
 Lot No. :E2086120F  
 Time Processed :9:36:40 AM  
 Month-Day-Year Processed :06/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm  
 Equipment:ZJ19010141

### <Chromatogram>

mV

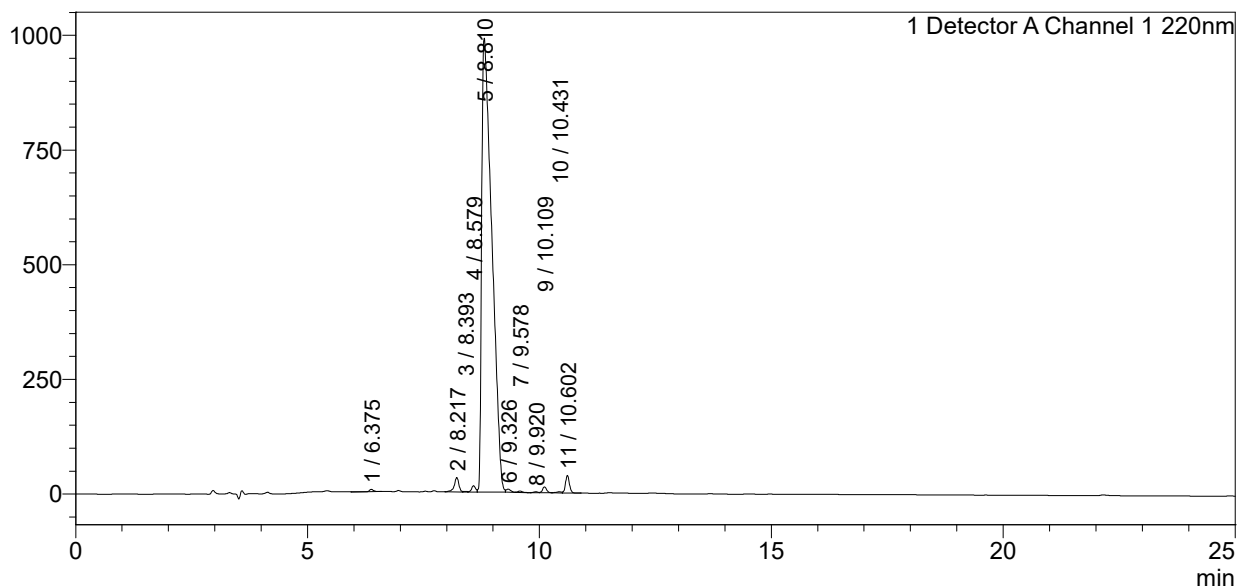

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.375	40583	5092	0.257
2	8.217	216684	31841	1.374
3	8.393	6965	1289	0.044
4	8.579	82699	13776	0.524
5	8.810	15018798	989862	95.246
6	9.326	44883	6858	0.285
7	9.578	16575	2746	0.105
8	9.920	12390	2056	0.079
9	10.109	79648	13005	0.505
10	10.431	21053	2454	0.134
11	10.602	228096	38517	1.447
Total		15768374	1107497	100.000