

Sample Name: Magainin 2
 Cat No.: RP11232
 Lot No.: E3978020I
 Time Processed: 11:08:47
 Month-Day-Year Processed :09/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

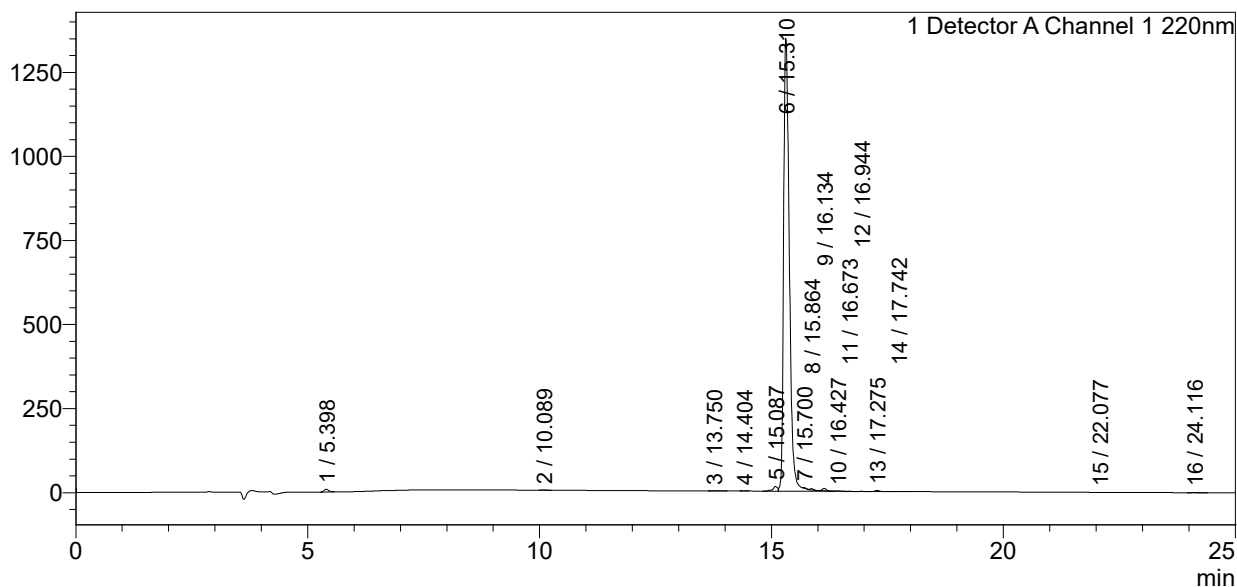

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.398	53418	8346	0.448
2	10.089	5327	989	0.045
3	13.750	2110	165	0.018
4	14.404	1212	232	0.010
5	15.087	102407	14167	0.859
6	15.310	11655700	1347765	97.744
7	15.700	7439	2059	0.062
8	15.864	15369	3408	0.129
9	16.134	43956	7333	0.369
10	16.427	7078	1228	0.059
11	16.673	2276	442	0.019
12	16.944	1778	335	0.015
13	17.275	20636	3308	0.173
14	17.742	2173	241	0.018
15	22.077	1008	130	0.008
16	24.116	2806	363	0.024

Peak#	Ret. Time	Area	Height	Area%
Total		11924692	1390510	100.000