

Sample Name :Gastrin-1, human  
 Cat No. :RP12740  
 Lot No. :E7918620L  
 Time Processed : 3:49:20 PM  
 Month-Day-Year Processed : 01/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

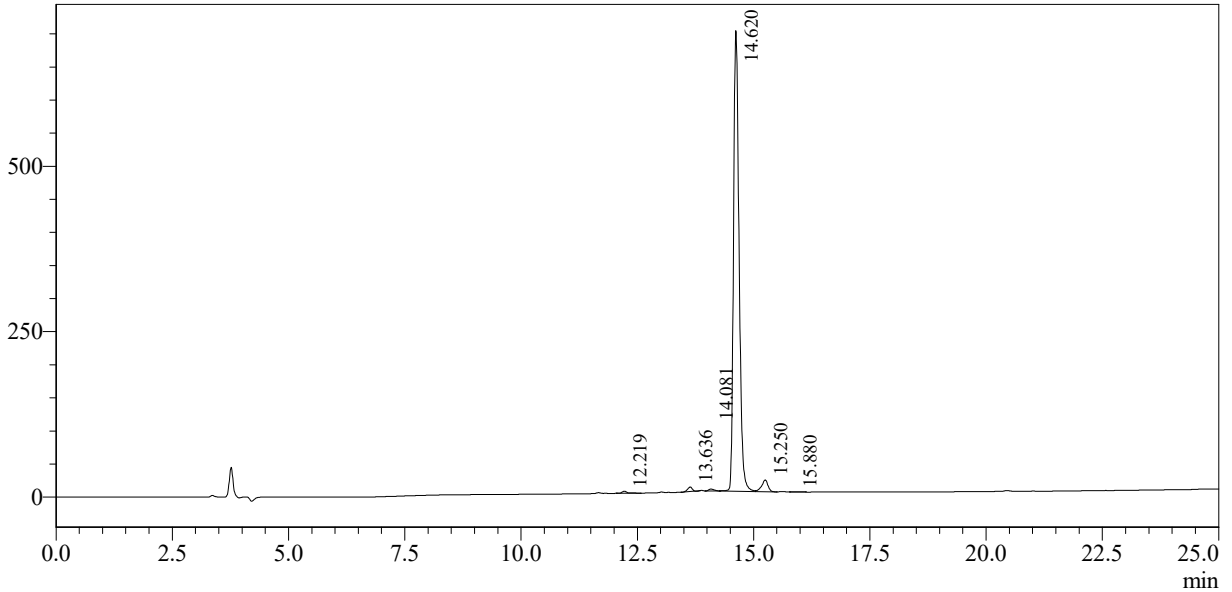

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.219	26992	3238	0.446
2	13.636	43217	6800	0.714
3	14.081	23796	2900	0.393
4	14.620	5787601	695912	95.622
5	15.250	166635	17766	2.753
6	15.880	4355	391	0.072
Total		6052595	727007	100.000