


Mass Spectrum

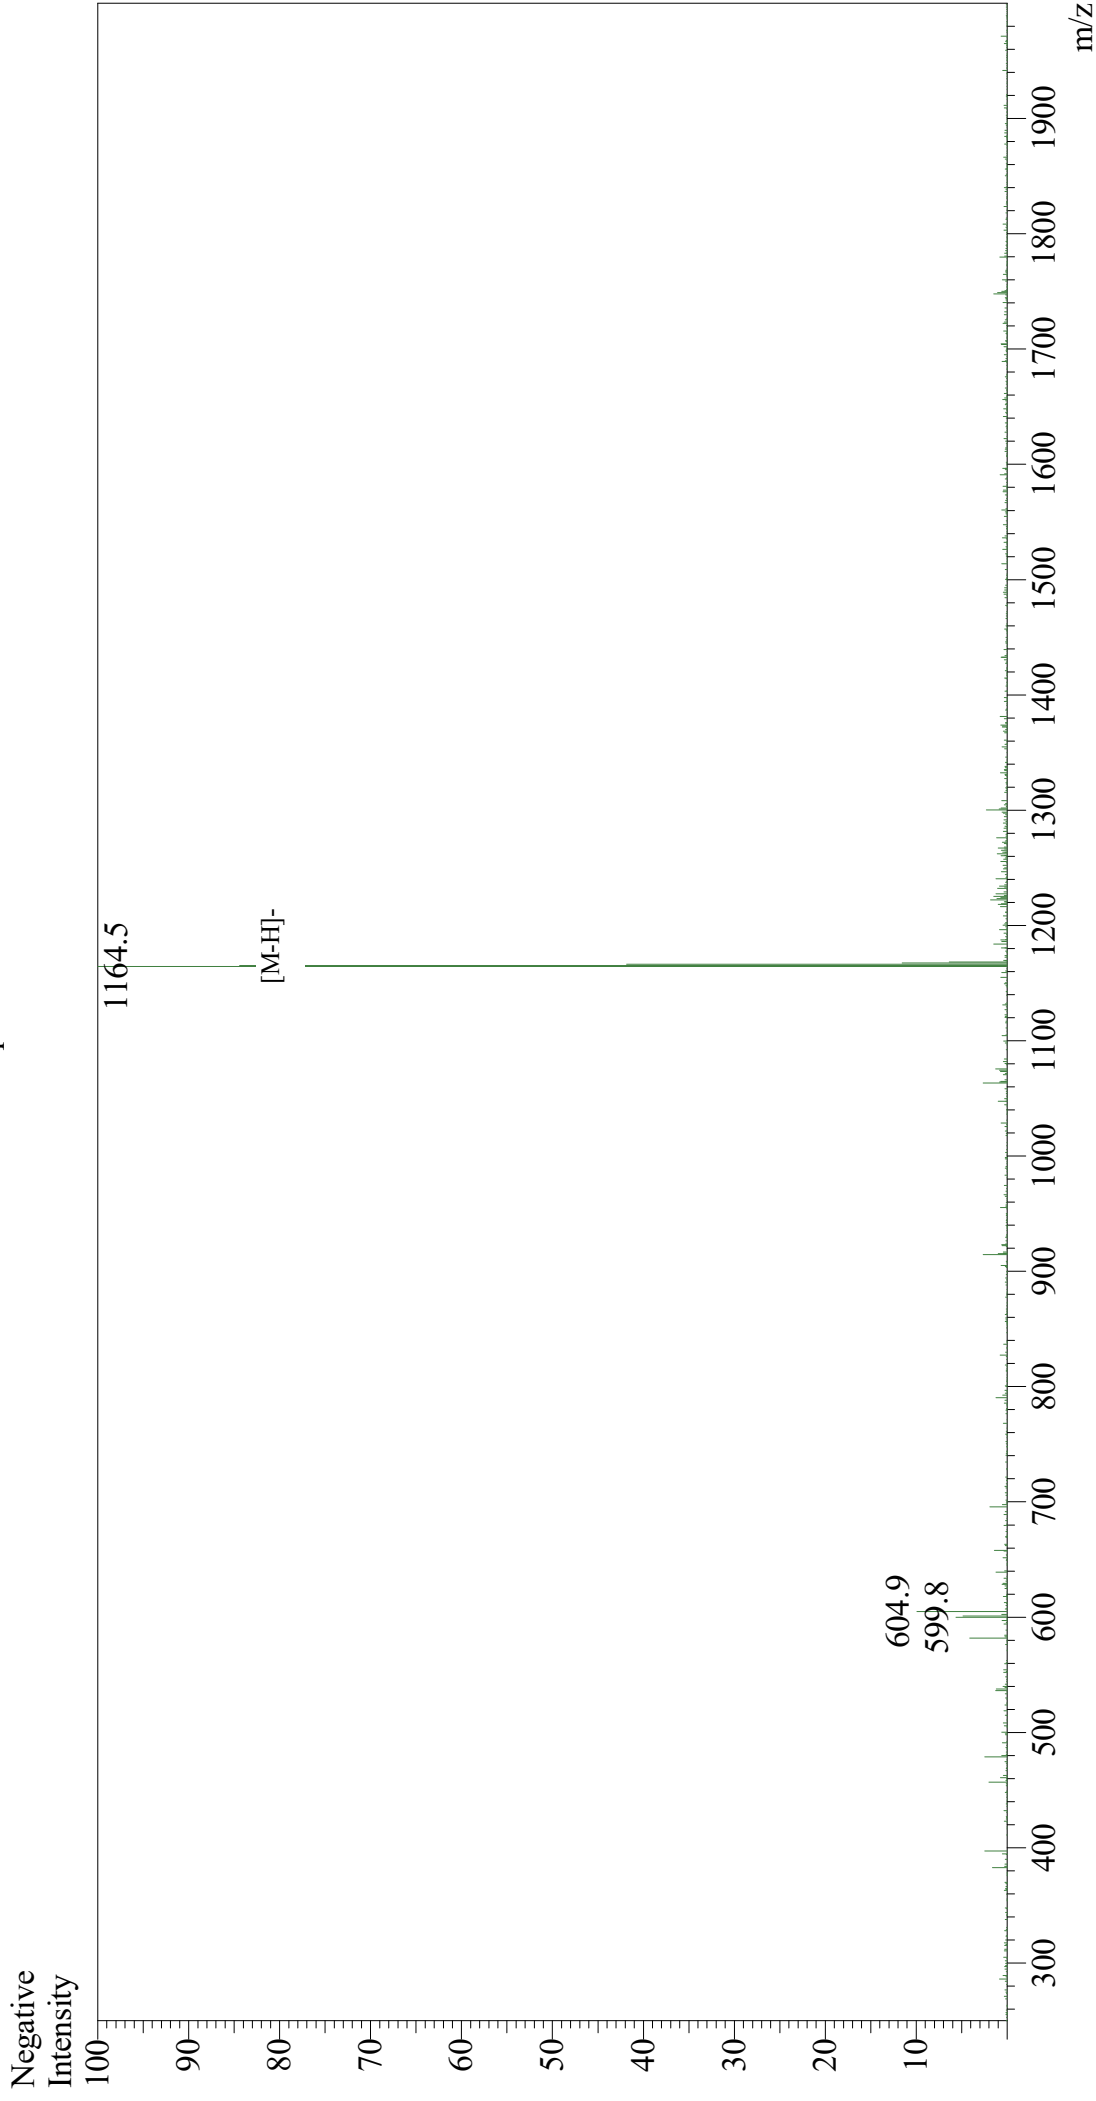

Sample Information

User : Gary
Month-Day Processed : 05/12/19
Time Processed : 09:57:10 AM
Injection Volume : 0.3
Sample Name : CTHWGFTLC, CYCLIC
Cat No. : RP20386
Lot No. : PE8821905
Theoretical MW : 1166.34
Observed MW : 1165.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : -3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH