

Sample Name :Biotin-TAT (47-57)
 Cat No :RP20408
 Lot No :E8175620L
 Time Processed :10:55:40 AM
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

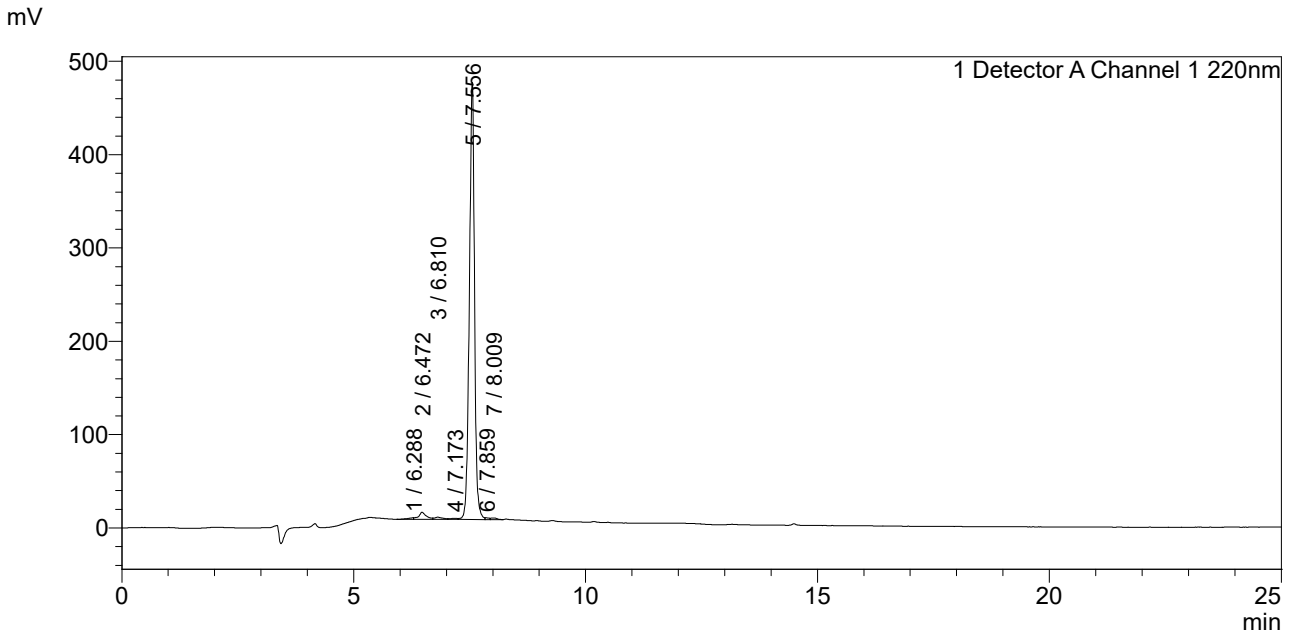

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.288	14646	1614	0.386
2	6.472	87139	7711	2.299
3	6.810	29181	2401	0.770
4	7.173	13053	1141	0.344
5	7.556	3620953	468254	95.523
6	7.859	10736	1906	0.283
7	8.009	14950	1724	0.394
Total		3790658	484751	100.000