

Sample Name :Phe-Met-Arg-Phe, amide
 Cat No. :RP10818
 Lot No. :E4424421A
 Time Processed :9:26:40 PM
 Month-Day-Year Processed :01/30/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

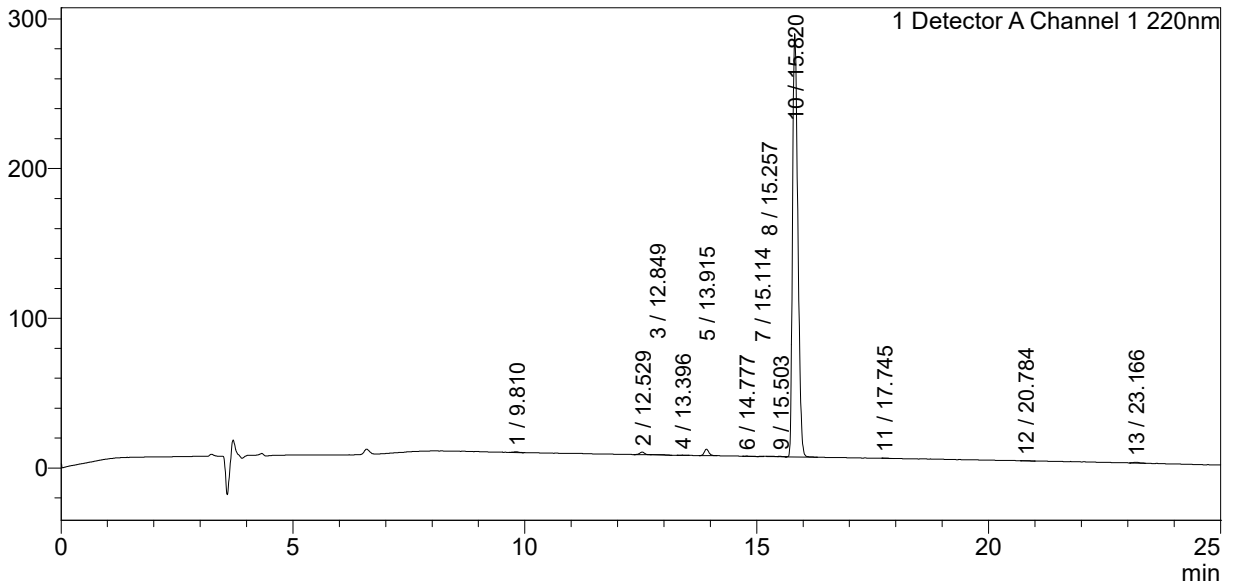

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.810	3917	510	0.168
2	12.529	12836	1774	0.551
3	12.849	4058	253	0.174
4	13.396	1123	130	0.048
5	13.915	30564	4372	1.313
6	14.777	1553	137	0.067
7	15.114	1168	223	0.050
8	15.257	3002	294	0.129
9	15.503	1592	261	0.068
10	15.820	2262631	282862	97.166
11	17.745	1176	120	0.050
12	20.784	1082	97	0.046
13	23.166	3912	417	0.168
Total		2328614	291452	100.000