

Sample Name :Neuropeptide AF (hNPAF), Human

Cat. No. : RP20315

Lot. No. : PE7381808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

### <Chromatogram>

mV

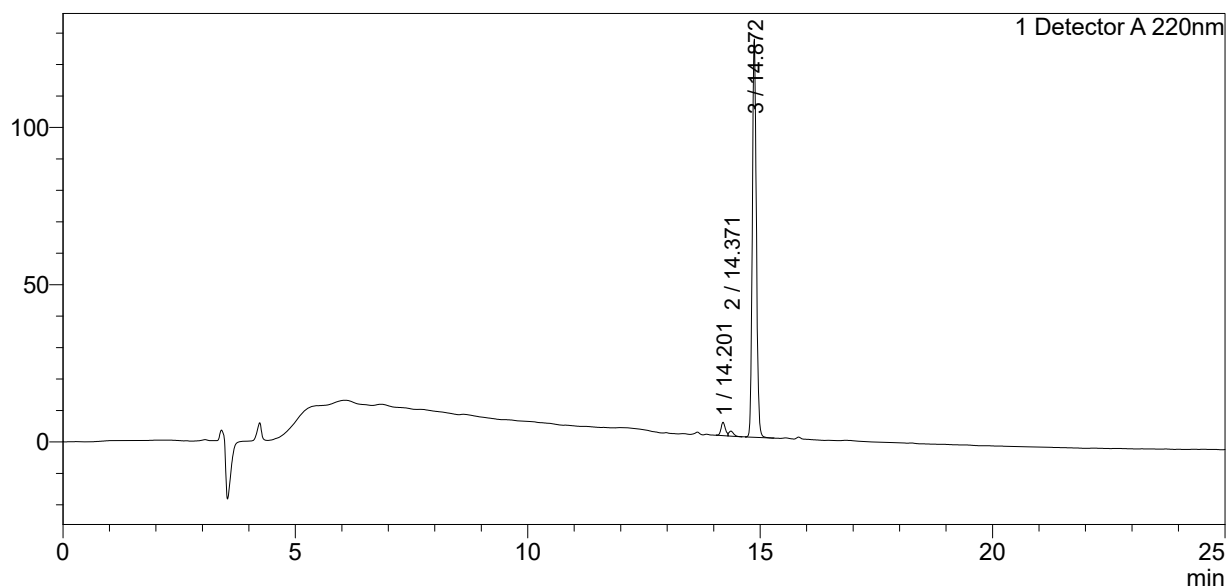

### <Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.201	27259	4251	3.386
2	14.371	10626	1593	1.320
3	14.872	767198	126611	95.294
Total		805083	132455	100.000