

Sample Name :Hexa-His
 Cat. No. : RP11737
 Lot. No. : E8197621C
 Time Processed :6:40:34 PM
 Month-Day-Year Processed :03/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

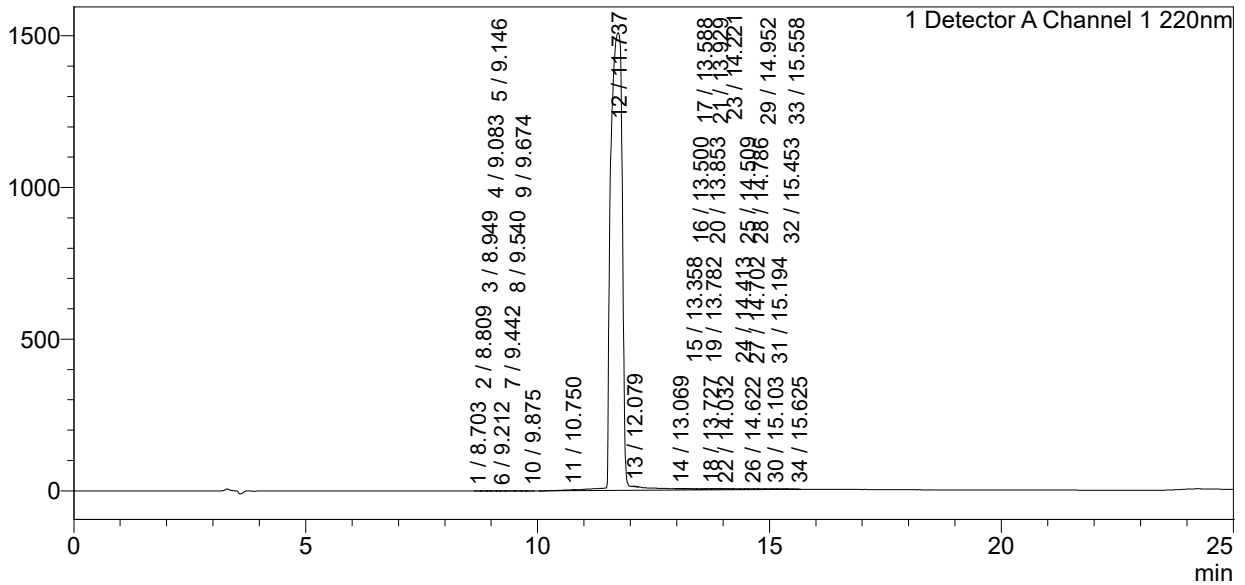

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.703	489	106	0.002
2	8.809	415	113	0.002
3	8.949	227	95	0.001
4	9.083	537	128	0.002
5	9.146	517	131	0.002
6	9.212	736	191	0.003
7	9.442	1179	209	0.004
8	9.540	899	151	0.003
9	9.674	307	103	0.001
10	9.875	303	65	0.001
11	10.750	61907	3052	0.233
12	11.737	26491092	1508882	99.533
13	12.079	8520	2208	0.032

Peak#	Ret. Time	Area	Height	Area%
14	13.069	1719	280	0.006
15	13.358	1829	77	0.007
16	13.500	160	72	0.001
17	13.588	917	259	0.003
18	13.727	2609	422	0.010
19	13.782	1501	460	0.006
20	13.853	2005	546	0.008
21	13.929	3519	628	0.013
22	14.032	7333	635	0.028
23	14.221	3414	418	0.013
24	14.413	2092	402	0.008
25	14.509	1388	350	0.005
26	14.622	3263	469	0.012
27	14.702	2320	507	0.009
28	14.786	3958	527	0.015
29	14.952	3643	445	0.014
30	15.103	1643	335	0.006
31	15.194	3575	394	0.013
32	15.453	915	182	0.003
33	15.558	308	96	0.001
34	15.625	222	91	0.001
Total		26615464	1523029	100.000