

Sample Name :Urotensin II, human
 Cat No.: RP10096
 Lot No.:E4689619I
 Time Processed:13:01:34
 Month-Day-Year Processed:09/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

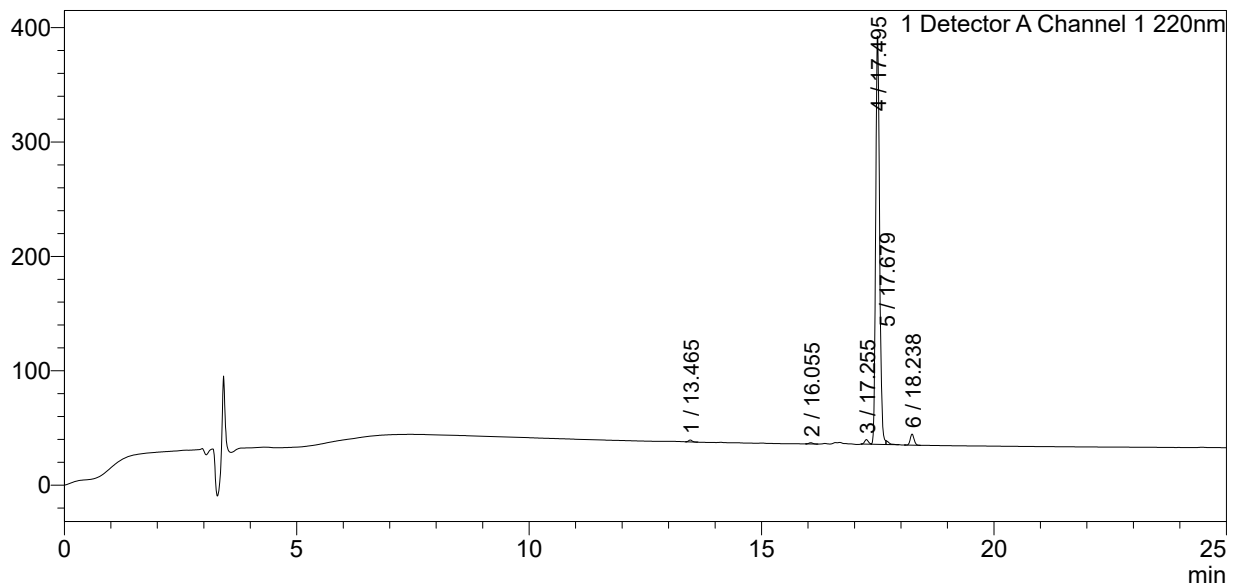

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.465	8758	1673	0.399
2	16.055	6775	1149	0.309
3	17.255	22845	3994	1.040
4	17.495	2087858	356945	95.095
5	17.679	14285	3372	0.651
6	18.238	55030	9628	2.506
Total		2195550	376760	100.000