

Sample Name :Bradykinin
Cat No. :RP11129
Lot No. :E0610920F
Time Processed :10:10:37 AM
Month-Day-Year Processed :06/19/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ17010508

<Chromatogram>

mV

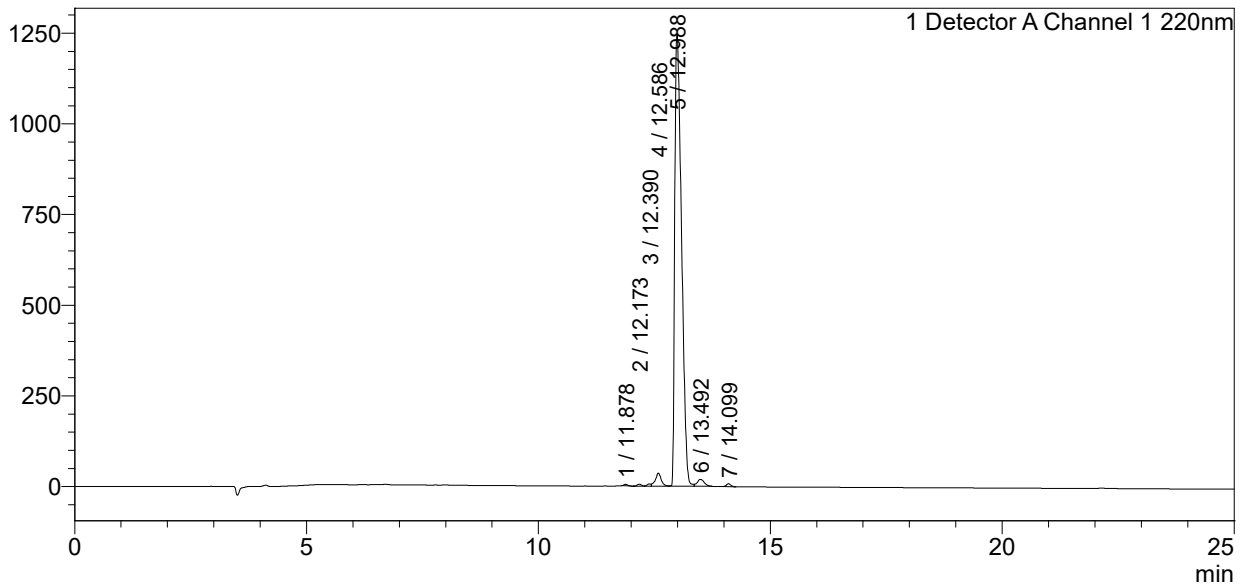

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.878	23060	4042	0.174
2	12.173	34646	5304	0.262
3	12.390	35448	6373	0.268
4	12.586	317373	35855	2.396
5	12.988	12585836	1246556	95.006
6	13.492	199264	18889	1.504
7	14.099	51853	7888	0.391
Total		13247478	1324907	100.000