

Sample Name :Arg-Gly-Asp-Cys
 Cat No. :RP10860
 Lot No. :E8019720I
 Time Processed :11:54:06 PM
 Month-Day-Year Processed :09/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

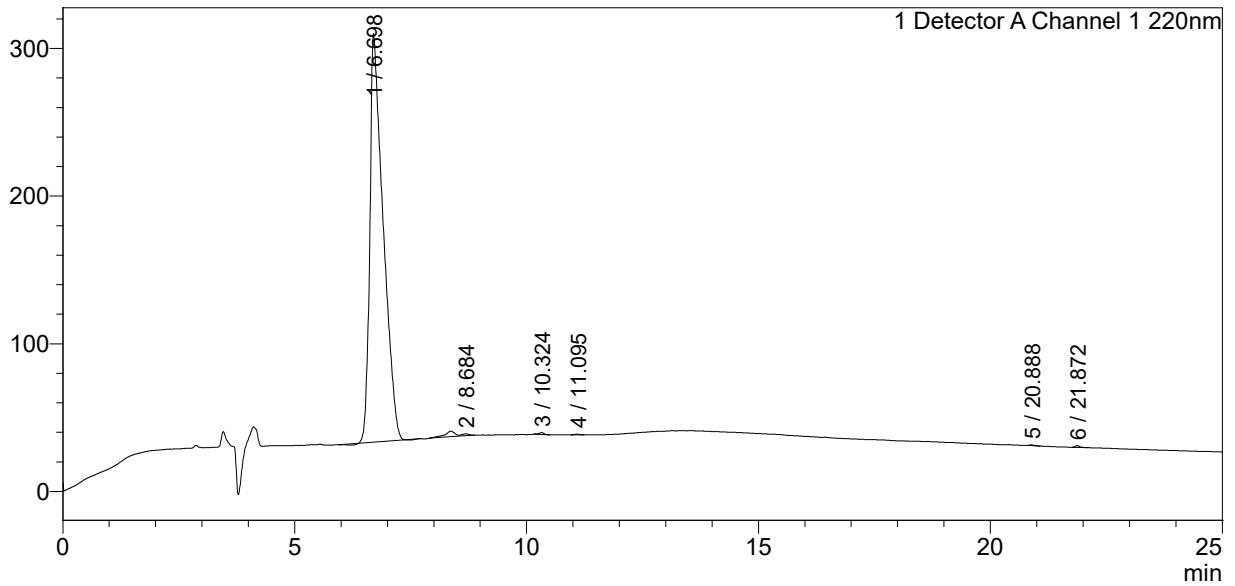

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.698	5516036	276679	98.278
2	8.684	72861	1267	1.298
3	10.324	9231	1229	0.164
4	11.095	3246	525	0.058
5	20.888	3127	557	0.056
6	21.872	8185	1251	0.146
Total		5612686	281509	100.000