

Sample Name : CEF6  
 Cat. No. : RP11768  
 Lot. No. : PE1301905  
 Time Processed : 10:52:27  
 Month-Day-Year Processed : 05/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

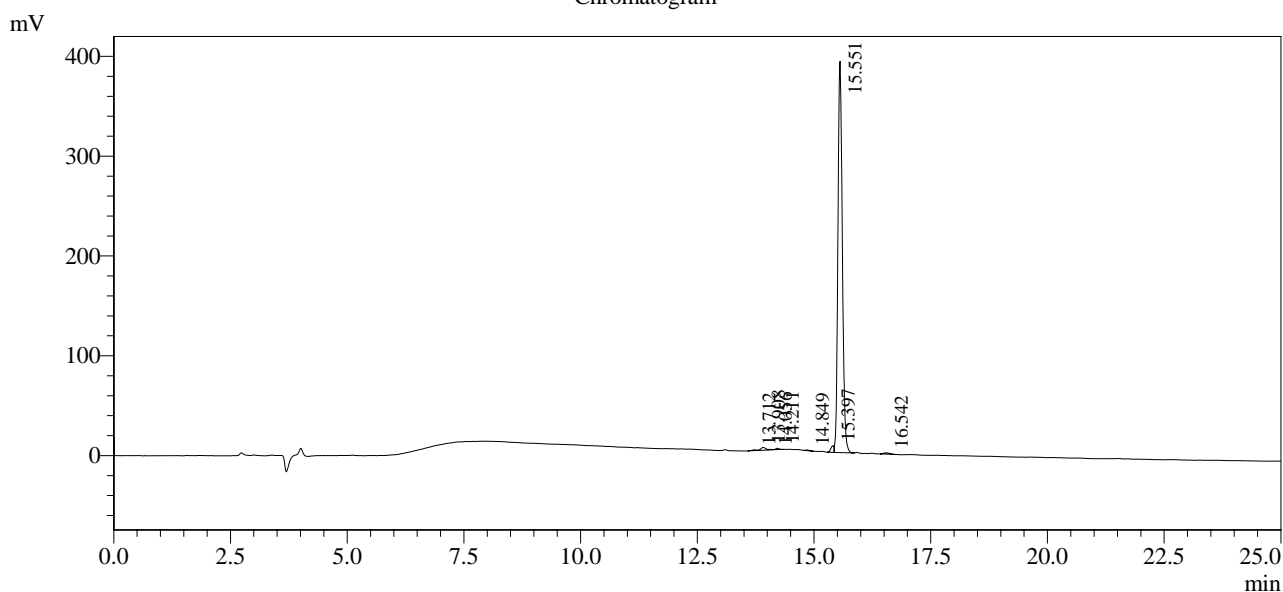

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.712	4755	771	0.179
2	13.908	20853	2845	0.785
3	14.056	2586	536	0.097
4	14.211	6763	1372	0.255
5	14.849	3084	645	0.116
6	15.397	32280	6520	1.216
7	15.551	2572535	392036	96.890
8	16.542	12240	1323	0.461
Total		2655096	406047	100.000