

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : PE7761904
 Time Processed :20:07:44
 Month-Day-Year Processed :04/12/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

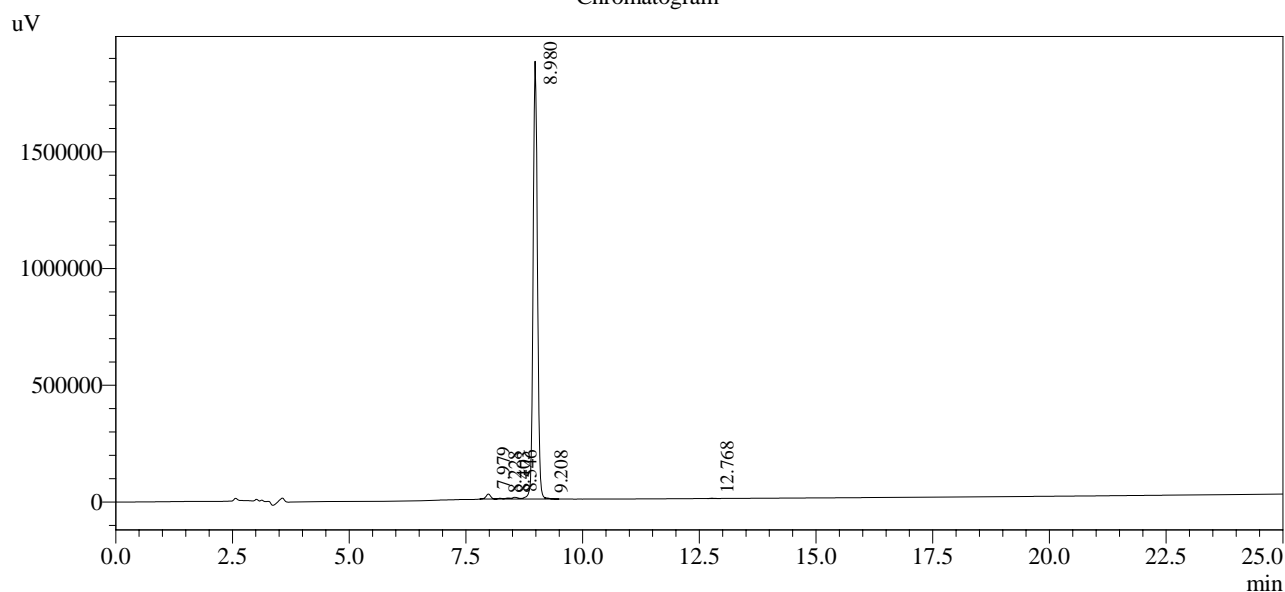

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.979	147319	21178	1.185
2	8.228	17811	3179	0.143
3	8.403	34460	4228	0.277
4	8.546	62243	7588	0.501
5	8.980	12135046	1875373	97.601
6	9.208	30516	5256	0.245
7	12.768	5891	1065	0.047
Total		12433286	1917867	100.000