

Sample Name :DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : E2914019G
 Time Processed : 10:18:13
 Month-Day-Year Processed : 07/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	15	
60.00	Pumps	Pump A B.Conc	95	
240.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

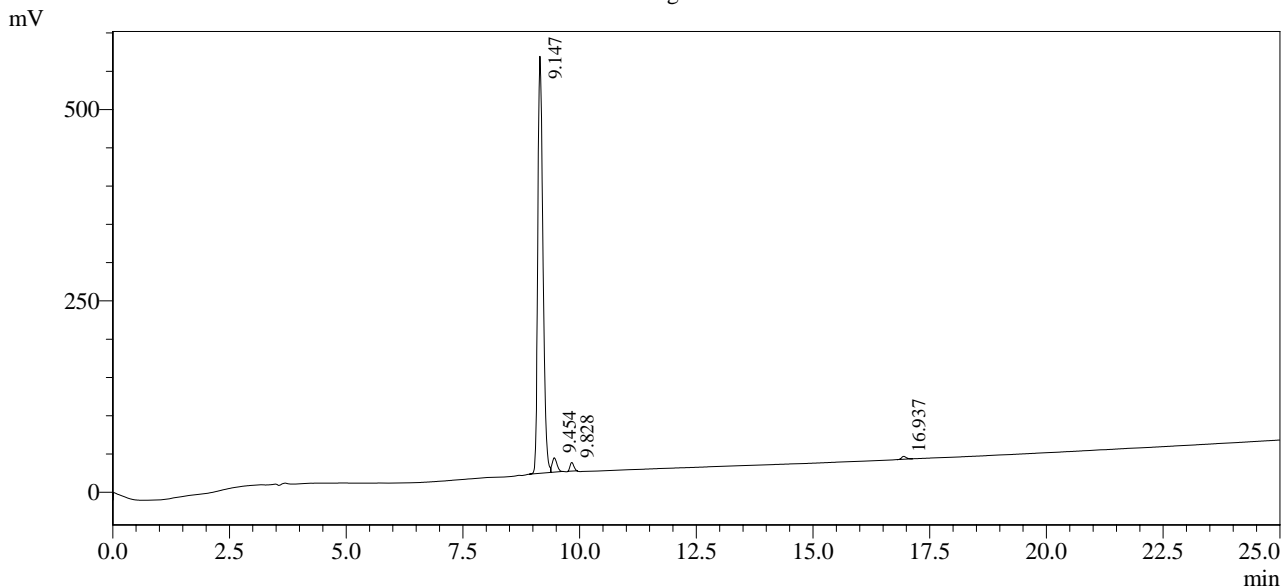

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.147	4217625	544892	95.027
2	9.454	130552	18715	2.941
3	9.828	63301	11260	1.426
4	16.937	26867	3859	0.605
Total		4438346	578727	100.000