

Sample Name : SIYRY  
 Cat. No. : RP20234  
 Lot. No. : PE0461612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

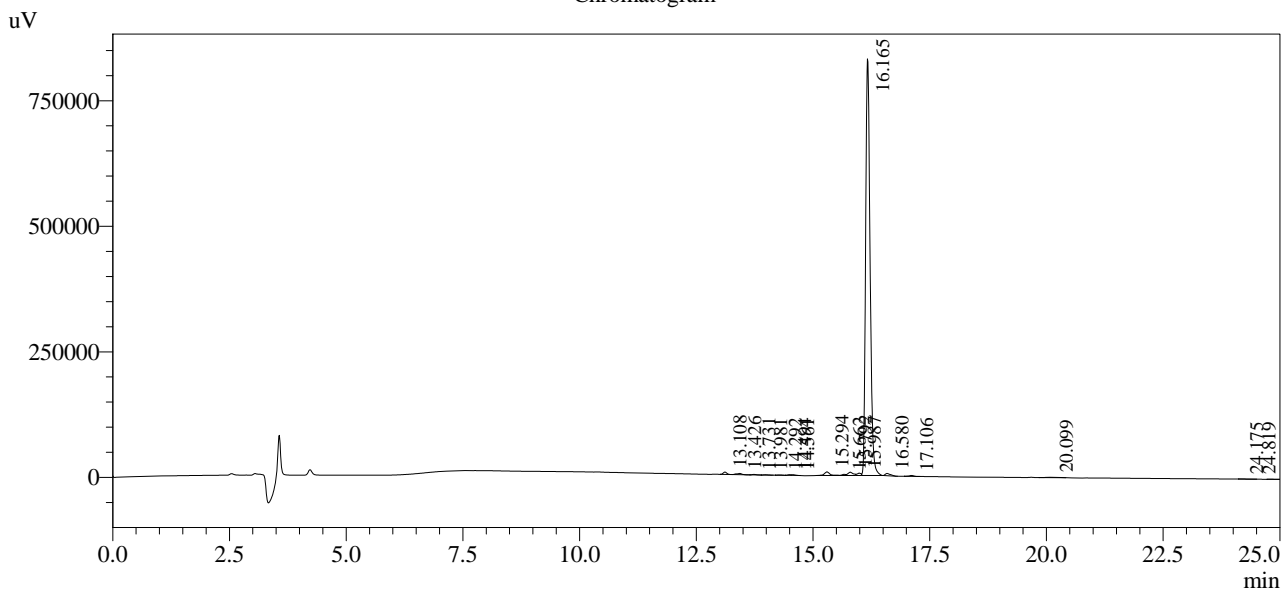

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.108	26034	4778	0.448
2	13.426	20359	2466	0.350
3	13.731	5711	1004	0.098
4	13.981	3349	595	0.058
5	14.292	2886	489	0.050
6	14.494	5896	1178	0.101
7	14.561	6185	1239	0.106
8	15.294	58953	7363	1.014
9	15.662	12538	2240	0.216
10	15.792	51885	6756	0.893
11	15.987	27440	4626	0.472
12	16.165	5526867	829609	95.091
13	16.580	34378	4450	0.591
14	17.106	12998	1863	0.224
15	20.099	14020	1185	0.241
16	24.175	1140	124	0.020
17	24.819	1519	197	0.026
Total		5812157	870163	100.000