

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : PE4201705

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

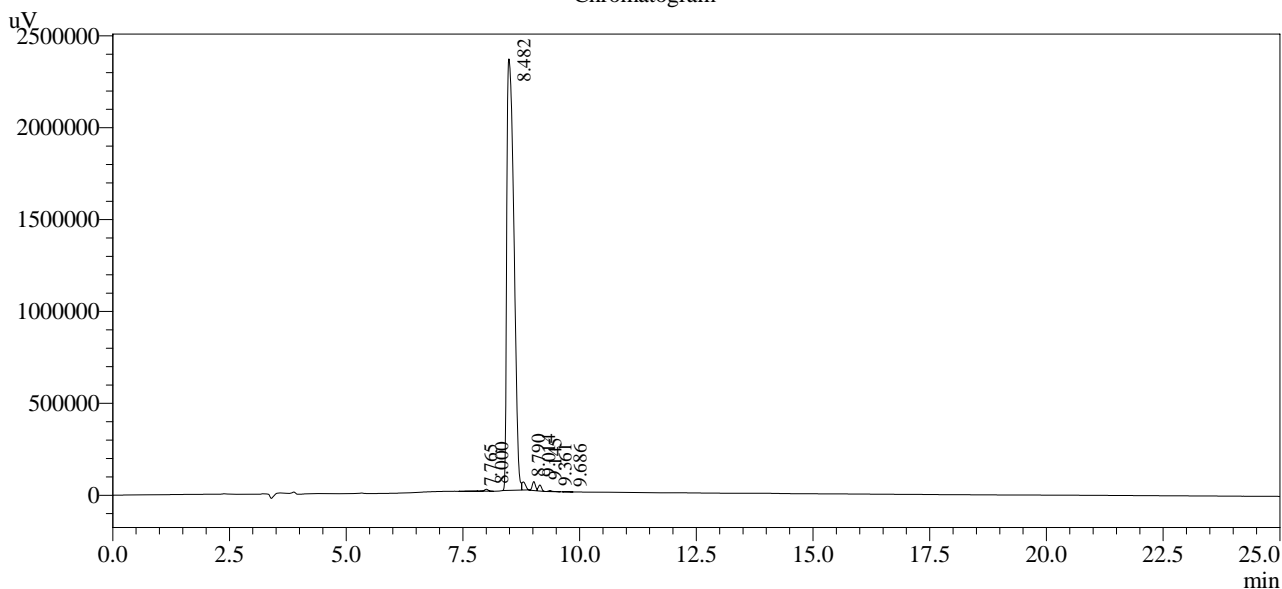

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.765	6147	656	0.024
2	8.000	64243	10391	0.250
3	8.482	24930210	2348428	97.181
4	8.790	227760	43764	0.888
5	9.014	235280	48713	0.917
6	9.145	155559	33526	0.606
7	9.361	32568	5624	0.127
8	9.686	1594	269	0.006
Total		25653362	2491372	100.000