

Sample Name :Axltime  
 Cat No.: RP20363  
 Lot No.:E6046820C  
 Time Processed :18:26:19  
 Month-Day-Year Processed :03/25/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

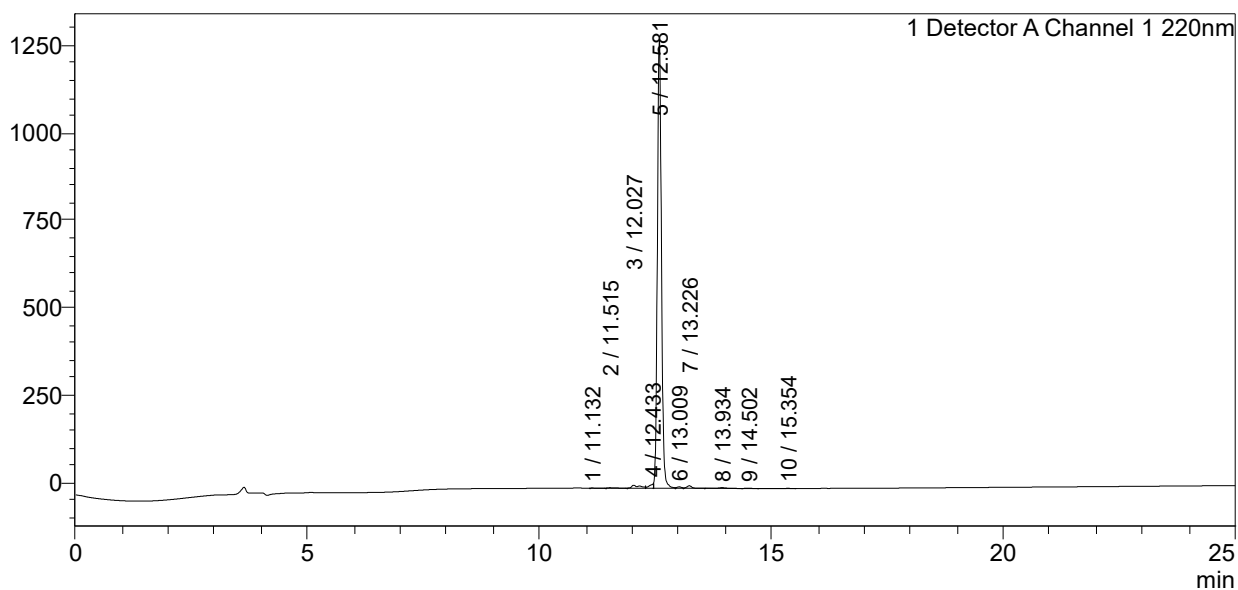

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.132	112	48	0.001
2	11.515	9982	1264	0.122
3	12.027	105430	8540	1.287
4	12.433	60411	10470	0.738
5	12.581	7907436	1282273	96.549
6	13.009	29879	4207	0.365
7	13.226	52220	7285	0.638
8	13.934	21225	1855	0.259
9	14.502	2529	461	0.031
10	15.354	817	93	0.010
Total		8190040	1316496	100.000