


Mass Spectrum

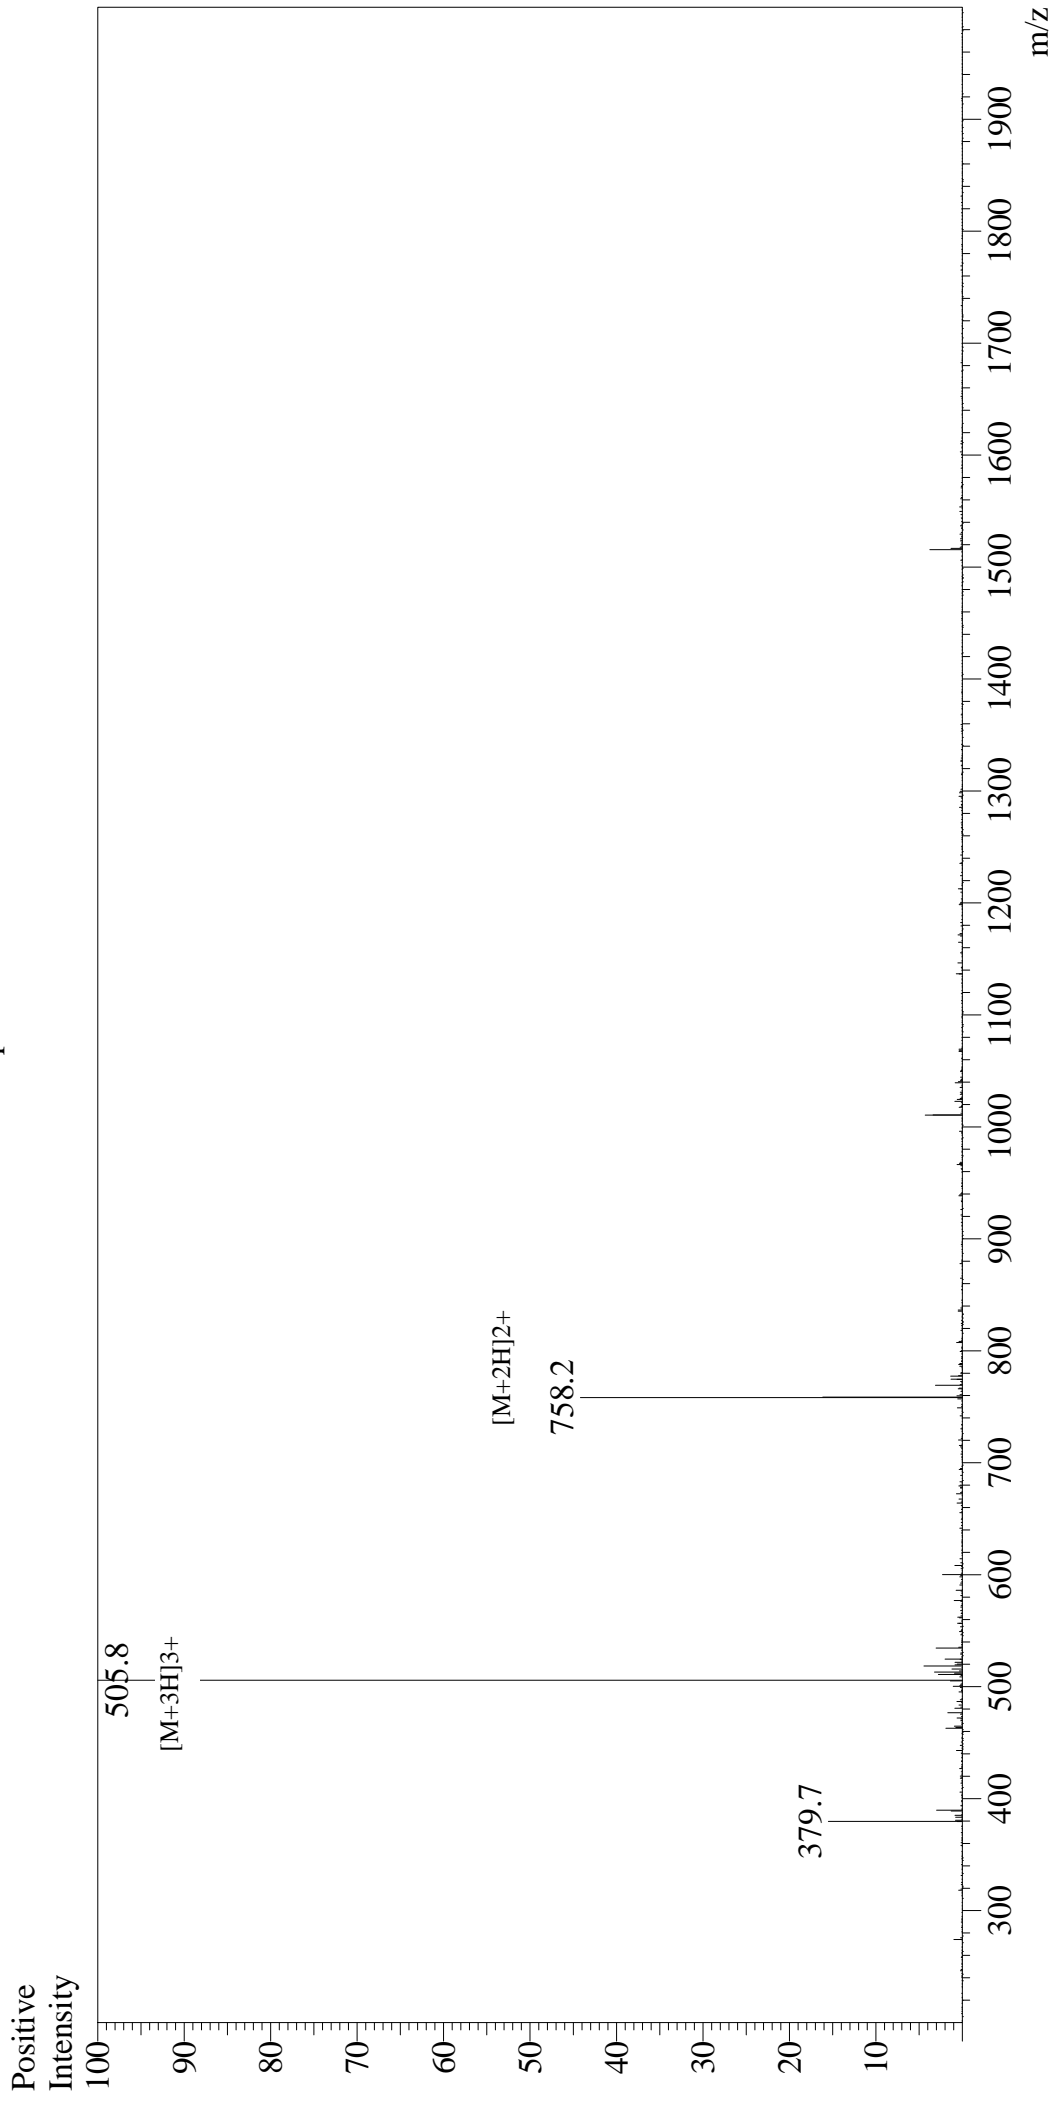

Sample Information

User : Gary
Month-Day Processed : 03/26/20
Time Processed : 19:39:04
Injection Volume : 0.6
Sample Name : Axltide
Cat No. : RP20363
Lot No. : E6046820C
Theoretical MW : 1514.78
Observed MW : 1514.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH