


Mass Spectrum

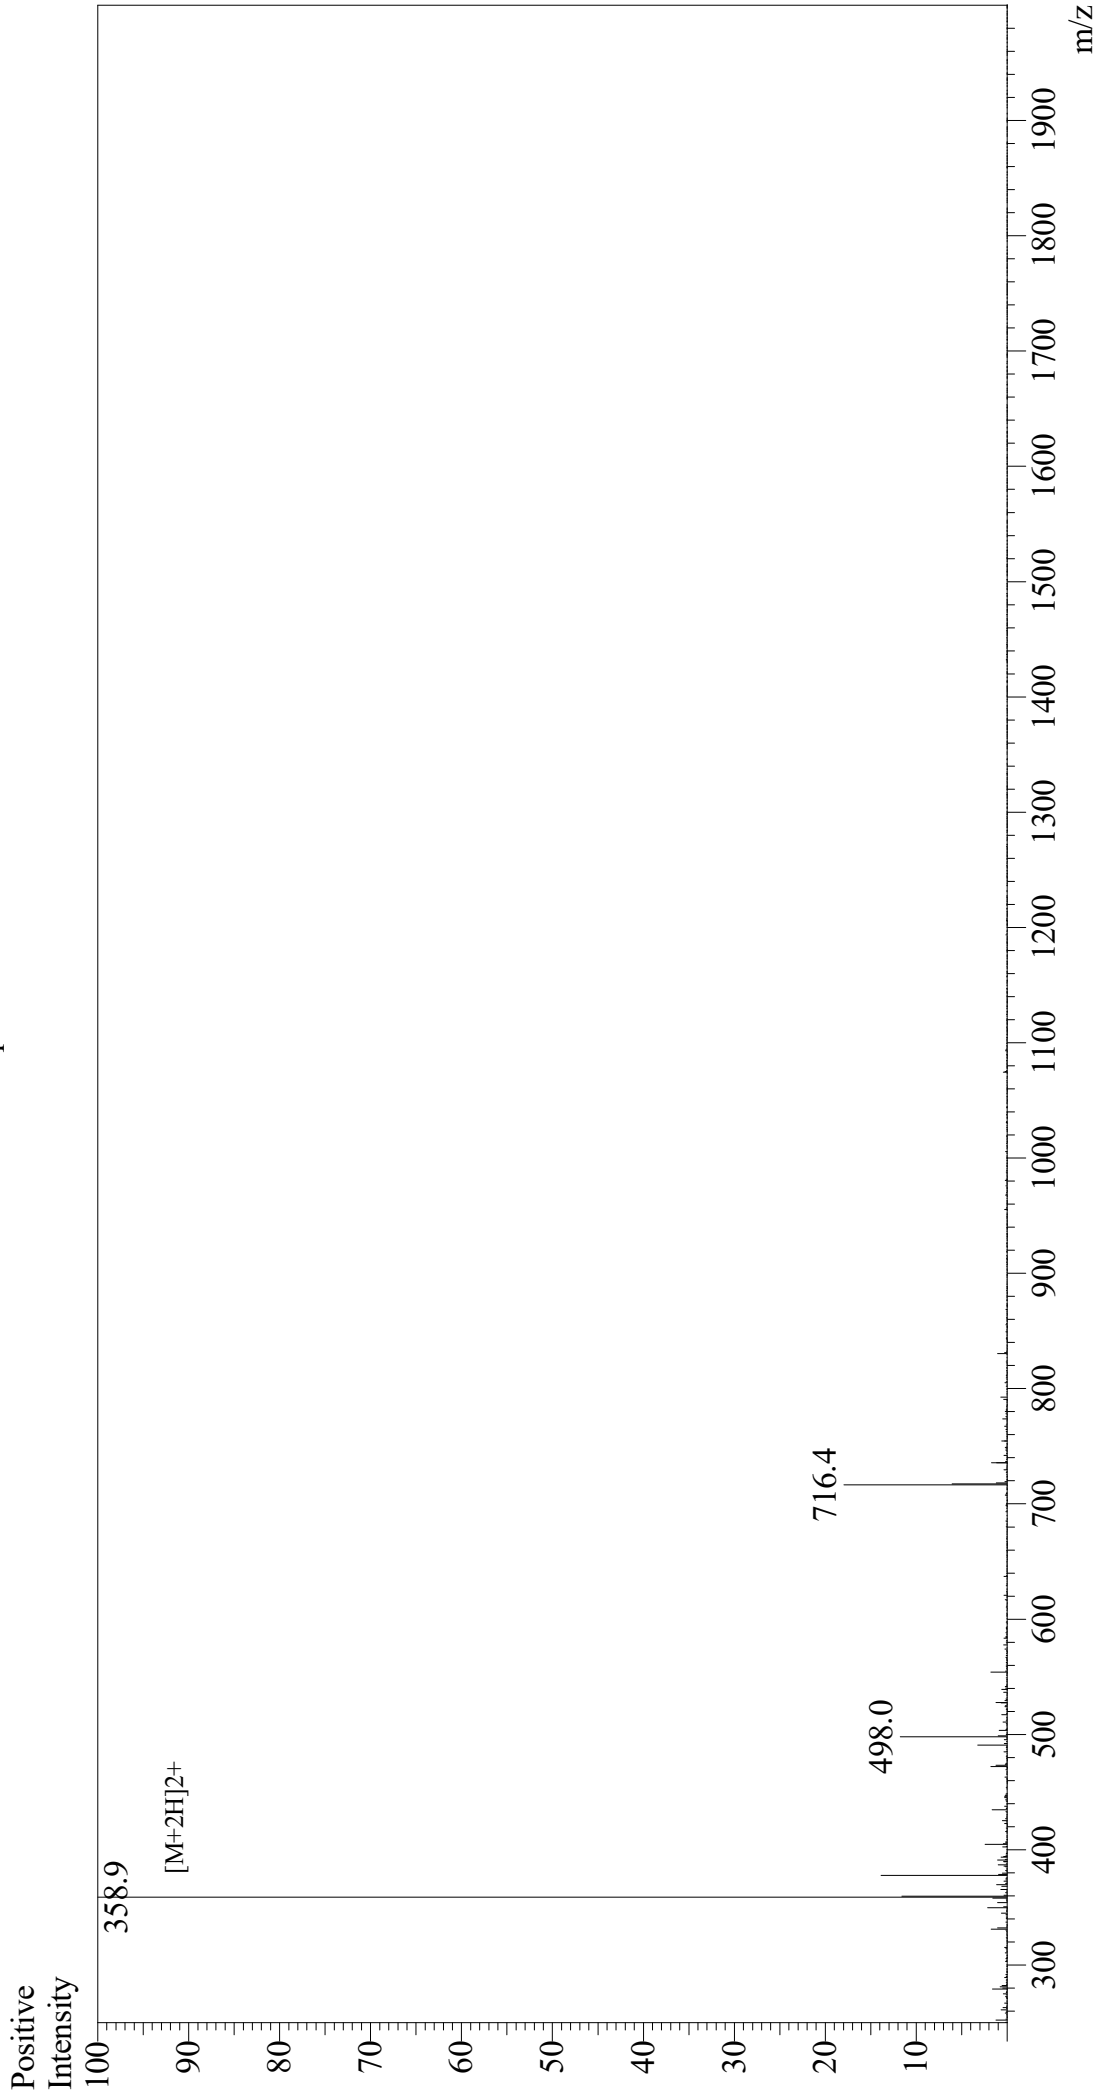

Sample Information
Month-Day/Processed : 03/11/21
Time Processed : 10:17:44 PM
Injection Volume : 0.4
Sample Name : GRGDSPK
Cat No. : RP20326
Lot No. : E808821C
Theoretical MW : 715.80
Observed MW : 715.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH