


# Mass Spectrum

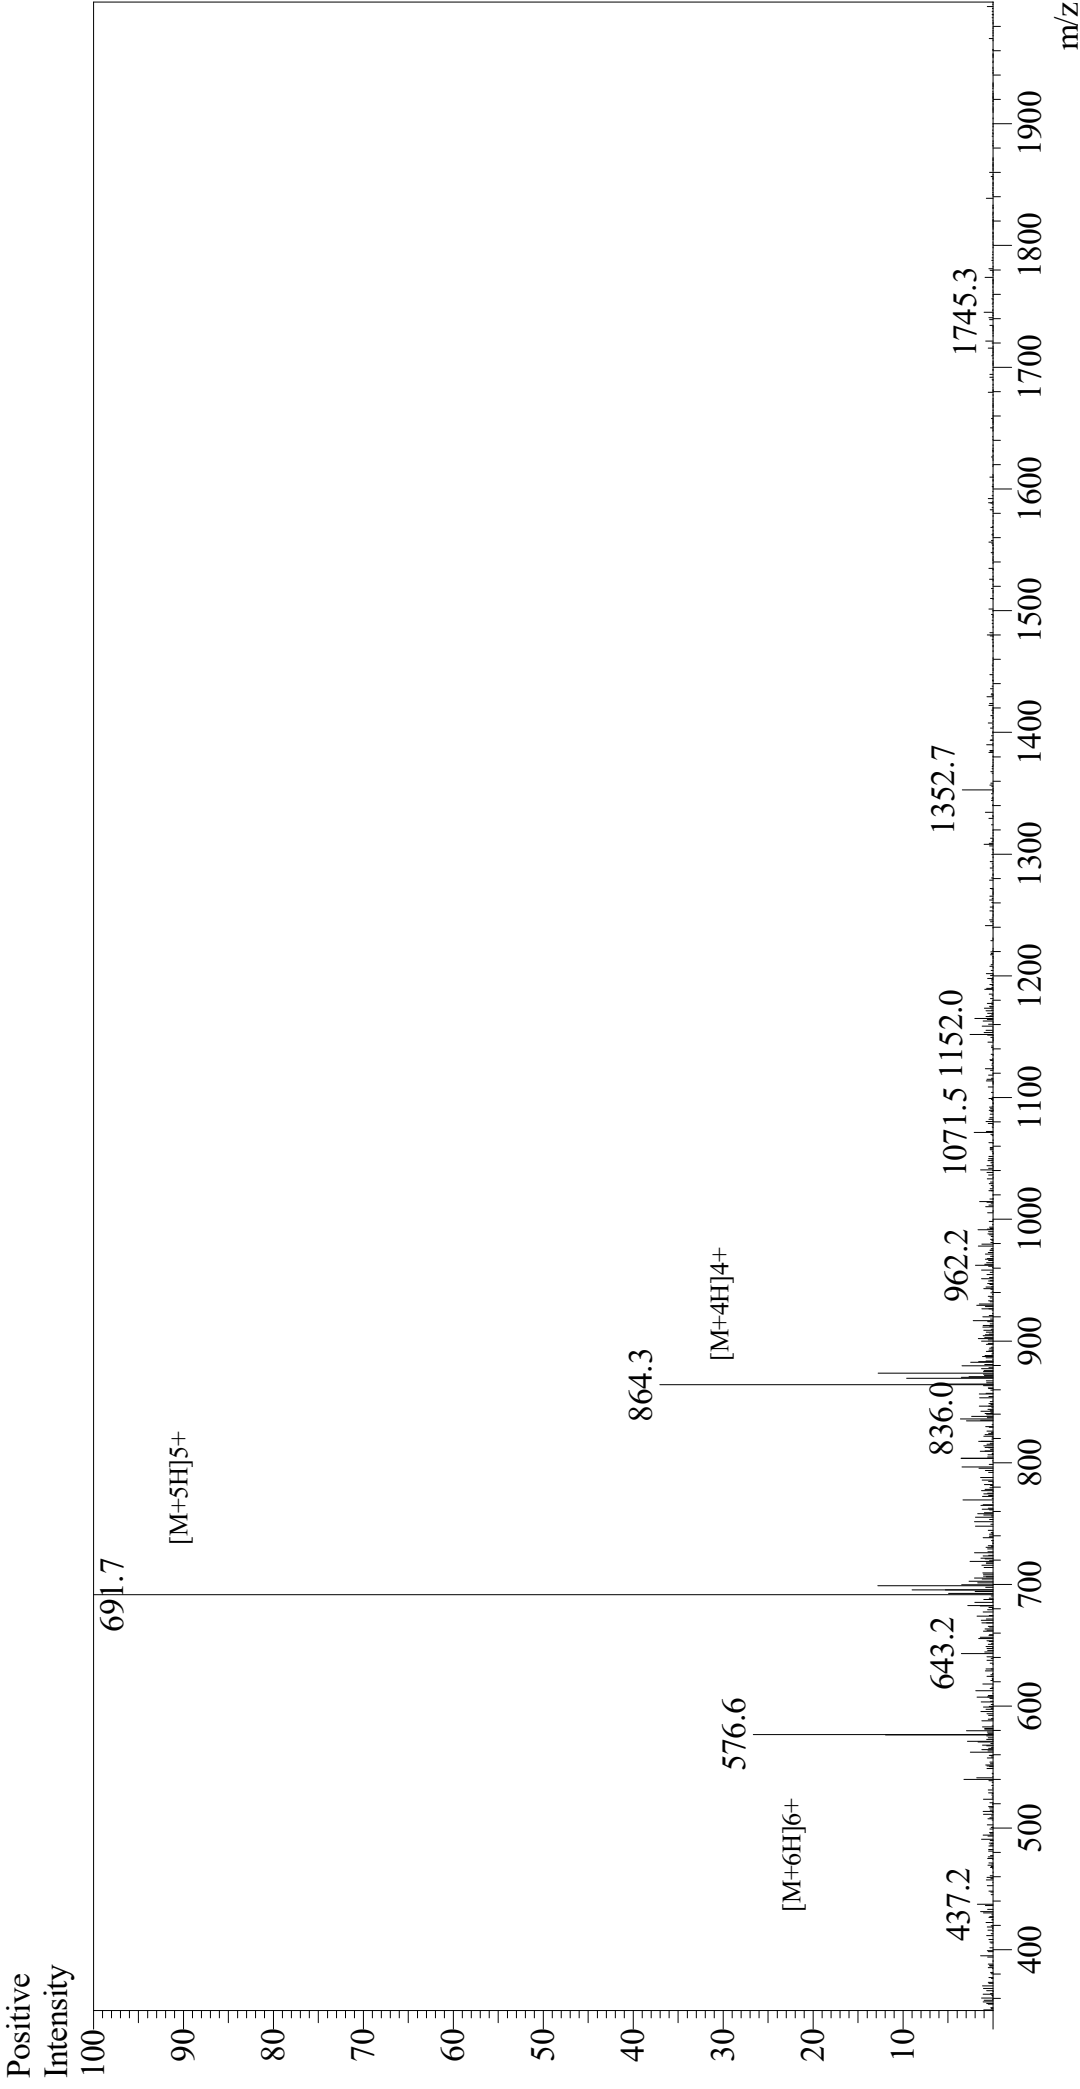

Sample Information	Interface	Equipment
Month-Day Processed : 05/13/21	Nebulizing Gas Flow : 1.5L/min	: GK11010007
Time Processed : 22:00:21	CDL Temp : 250	Interface Bias : +4.5 kV
Injection Volume : 0.2	Block Temp : 200	Drying Gas Flow : 5 L/min
Sample Name : Brain Natriuretic Peptide (BNP) (1-32), rat		T.Flow : 0.2 ml/min
Cat No : RP11121		B.conc : 50% H2O/50% MeOH
Lot No : E2526621D		
Theoretical MW : 3452.94		
Observed MW : 3453.5		