

Sample Name :MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E0909519G
 Time Processed : 7:41:31
 Month-Day-Year Processed : 07/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

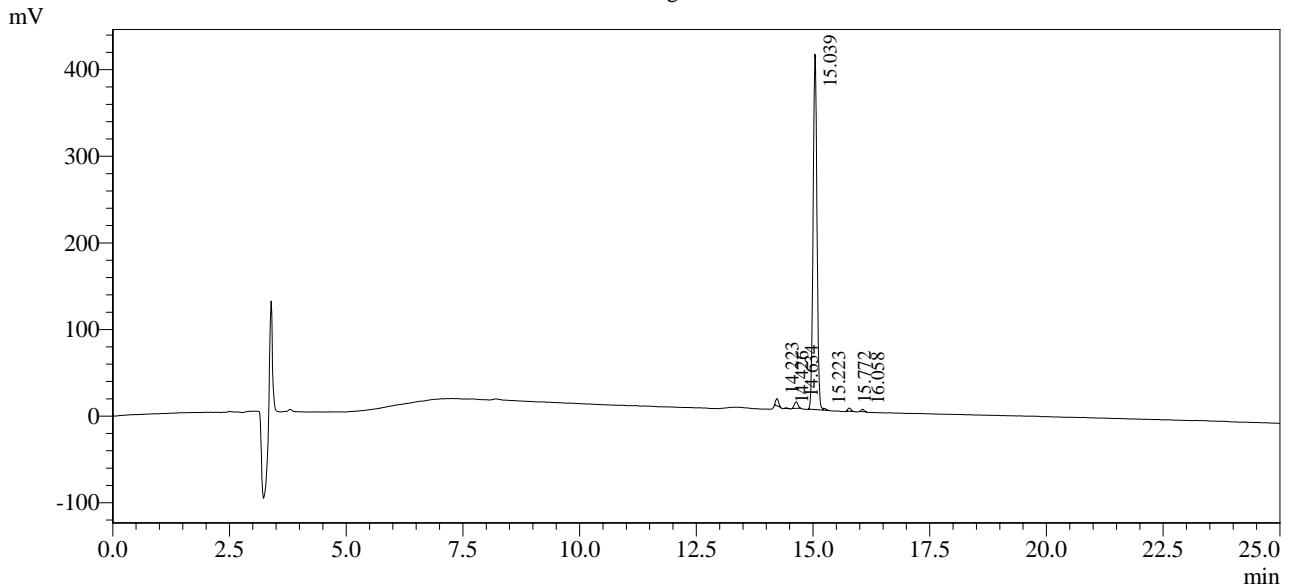

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.223	34587	8257	1.397
2	14.426	1959	516	0.079
3	14.634	40485	7479	1.635
4	15.039	2361775	410245	95.408
5	15.223	8477	2030	0.342
6	15.772	16406	3677	0.663
7	16.058	11761	2714	0.475
Total		2475451	434919	100.000