

Sample Name : Angiotensin II, human
 Cat. No. : RP11257
 Lot. No. : E6861520A
 Time Processed :8:03:41
 Month-Day-Year Processed :01/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

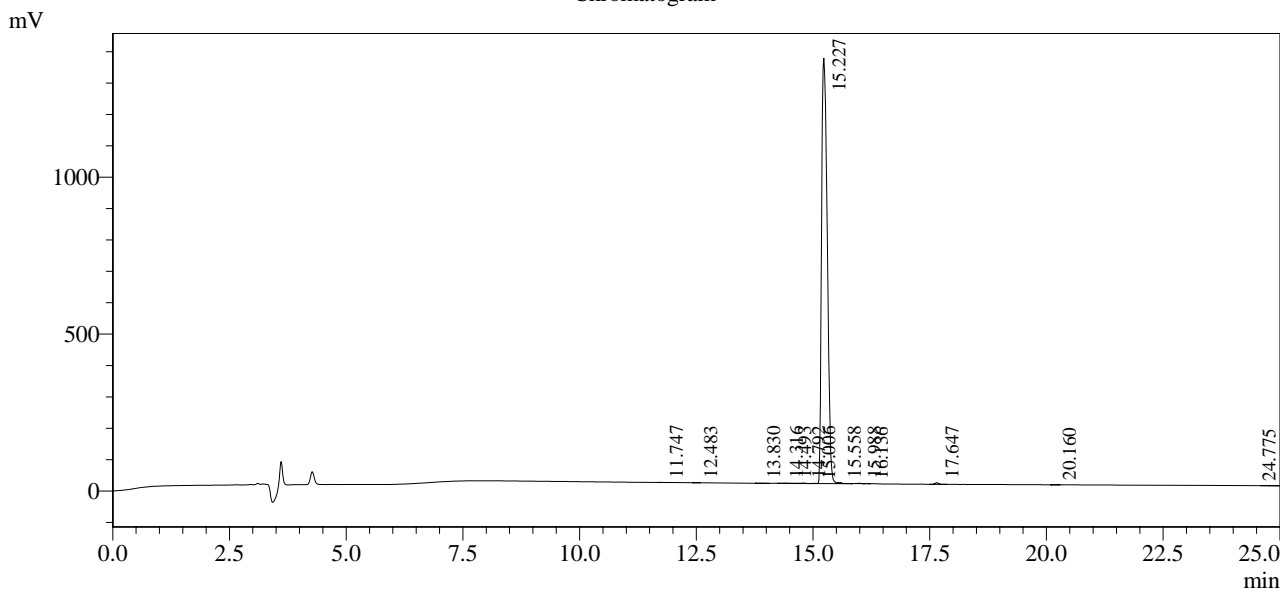

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.747	1692	306	0.015
2	12.483	1572	360	0.014
3	13.830	2454	359	0.021
4	14.316	2001	399	0.017
5	14.493	3270	614	0.028
6	14.792	10157	1432	0.088
7	15.006	2457	495	0.021
8	15.227	11534490	1355280	99.455
9	15.558	2188	678	0.019
10	15.988	5147	1093	0.044
11	16.136	1398	358	0.012
12	17.647	27343	4900	0.236
13	20.160	1105	185	0.010
14	24.775	2476	192	0.021
Total		11597751	1366651	100.000