

Sample Name :PUMA BH3
 Cat No. :RP20510
 Lot No. :E4942219I
 Time Processed :12:42:42 PM
 Month-Day-Year Processed :09/29/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

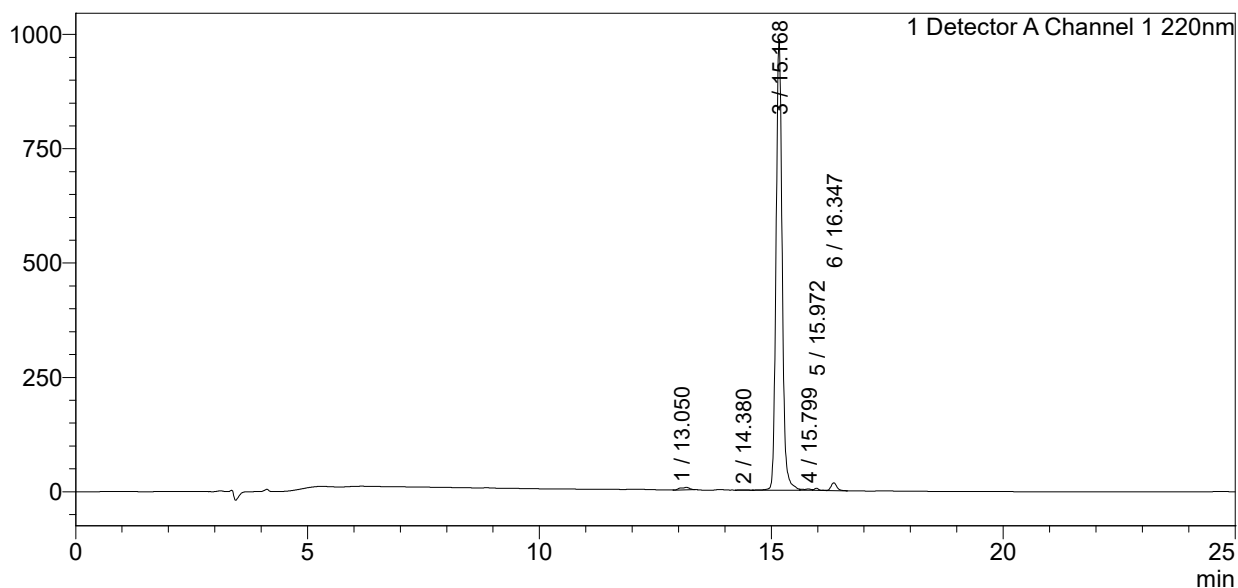

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.050	76481	4444	0.818
2	14.380	15151	1066	0.162
3	15.168	9046025	986999	96.724
4	15.799	39147	3310	0.419
5	15.972	31989	4867	0.342
6	16.347	143619	16957	1.536
Total		9352411	1017644	100.000