

Sample Name : SIYRY
 Cat. No. : RP20234
 Lot. No. : PE7691712

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

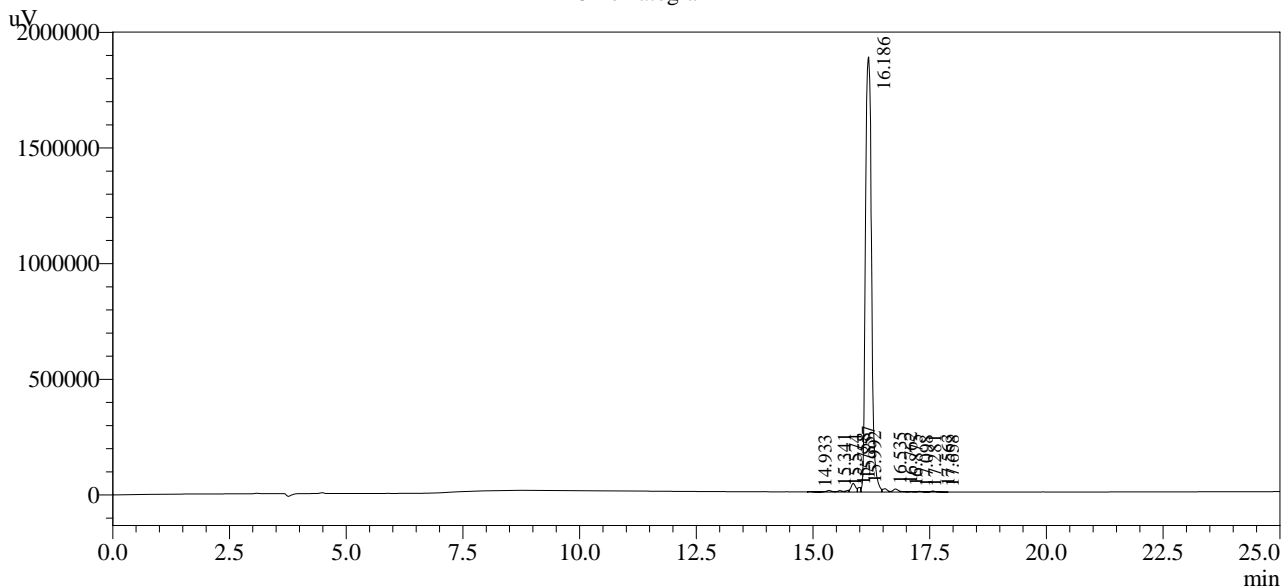

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.933	6011	1183	0.034
2	15.341	53263	6493	0.302
3	15.574	45873	5818	0.260
4	15.758	31129	7171	0.176
5	15.857	260019	37233	1.474
6	15.992	81977	19428	0.465
7	16.186	16870723	1881105	95.630
8	16.535	96969	14273	0.550
9	16.762	102819	12989	0.583
10	16.875	16184	3168	0.092
11	17.098	17254	1865	0.098
12	17.281	23156	2937	0.131
13	17.563	29730	4377	0.169
14	17.658	6463	1249	0.037
Total		17641573	1999290	100.000