

Sample Name :InsB 9-23
 Cat. No. : RP20391
 Lot. No. : PE7201710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

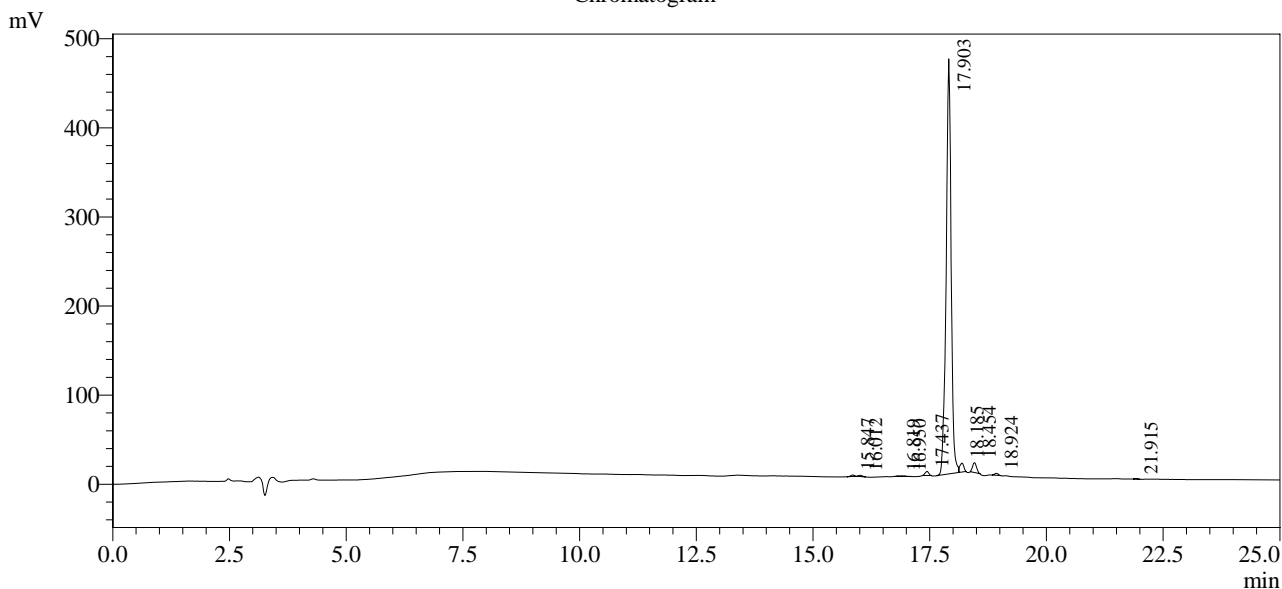

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.847	8326	1556	0.228
2	16.012	7462	1489	0.204
3	16.819	2271	469	0.062
4	16.950	1049	305	0.029
5	17.437	24180	4622	0.662
6	17.903	3471871	466033	95.067
7	18.185	58077	10108	1.590
8	18.454	65388	11017	1.790
9	18.924	11791	2122	0.323
10	21.915	1601	391	0.044
Total		3652018	498113	100.000