

Sample Name :[Met5]-Enkephalin
 Cat No. :RP10886
 Lot No. :E7714620H
 Time Processed :15:53:27
 Month-Day-Year Processed :08/12/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

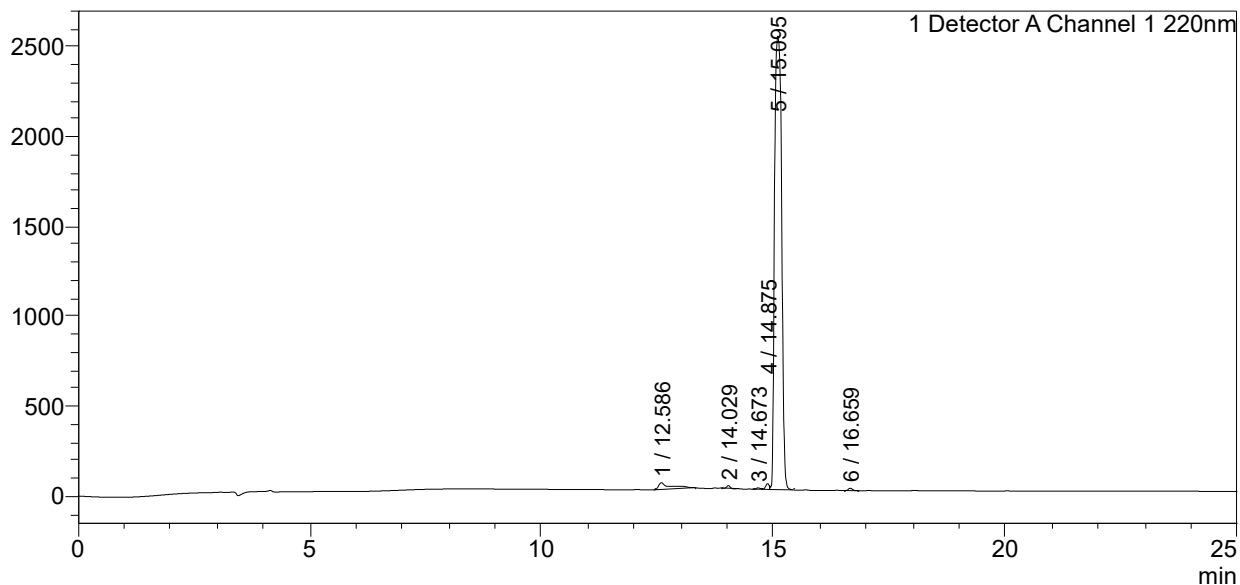

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.586	683850	37233	2.481
2	14.029	50783	14281	0.184
3	14.673	49250	8234	0.179
4	14.875	186769	31910	0.677
5	15.095	26515446	2522737	96.179
6	16.659	82719	12916	0.300
Total		27568817	2627310	100.000