

Sample Name : Gastrin-1, human
 Cat. No. : RP12740
 Lot. No. : PE9561803

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	15	
35.00	Pumps	Pump A B.Conc	15	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

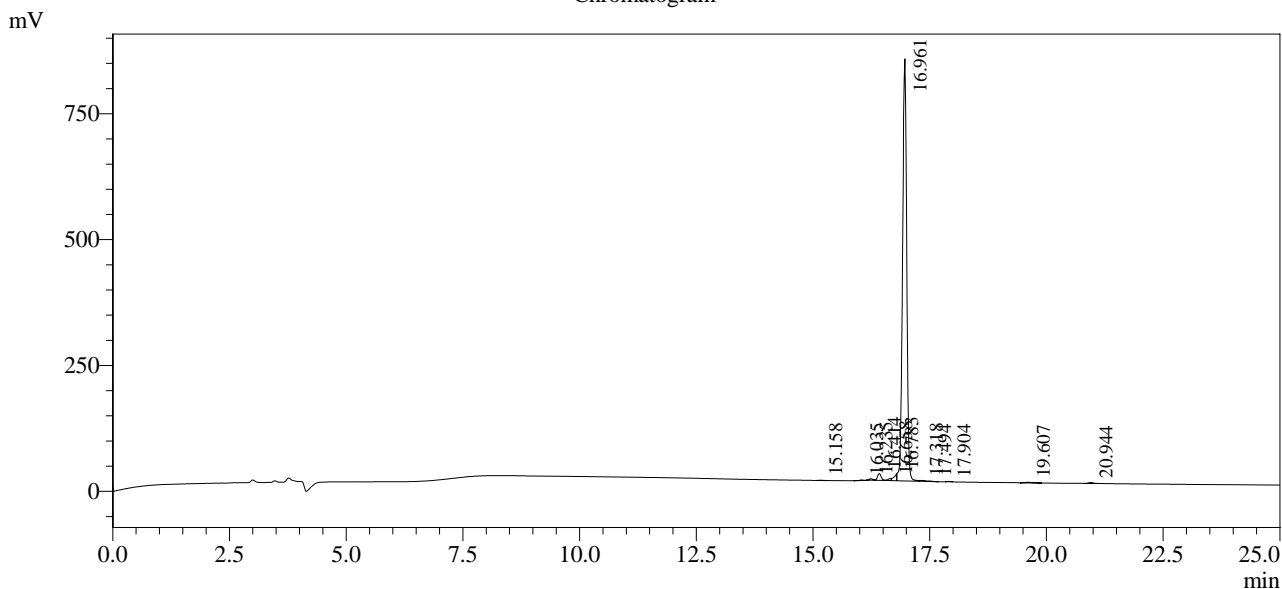

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.158	3009	564	0.055
2	16.035	5878	1267	0.108
3	16.235	15155	2991	0.279
4	16.414	73454	13438	1.350
5	16.658	19681	4356	0.362
6	16.783	57040	13090	1.049
7	16.961	5215513	838453	95.874
8	17.318	15865	1867	0.292
9	17.494	8233	1131	0.151
10	17.904	3069	634	0.056
11	19.607	9085	1236	0.167
12	20.944	13995	1867	0.257
Total		5439978	880894	100.000