

Sample Name : Proctolin  
 Cat. No. : RP10475  
 Lot. No. : E3873020G  
 Time Processed : 1:17:57  
 Month-Day-Year Processed : 07/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

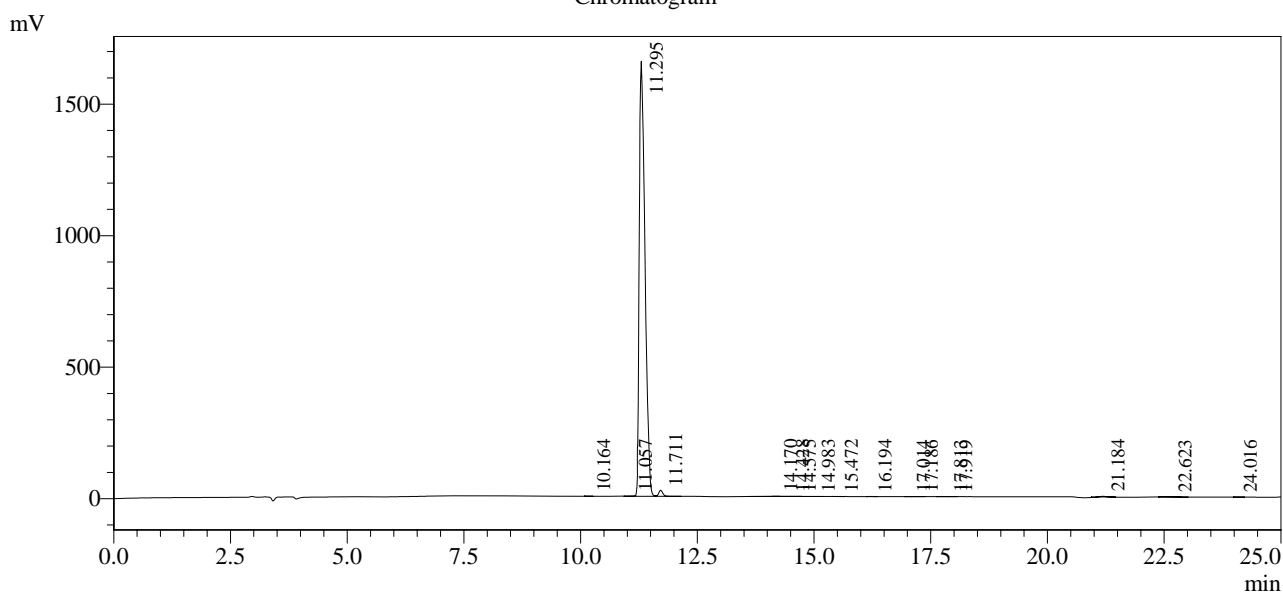

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.164	1222	214	0.008
2	11.057	3933	591	0.027
3	11.295	14148050	1654085	98.336
4	11.711	138129	22872	0.960
5	14.170	30764	1342	0.214
6	14.428	6866	840	0.048
7	14.575	11626	723	0.081
8	14.983	2118	264	0.015
9	15.472	1677	239	0.012
10	16.194	2059	268	0.014
11	17.014	1022	156	0.007
12	17.186	3089	333	0.021
13	17.813	1056	147	0.007
14	17.919	1142	153	0.008
15	21.184	18583	2377	0.129
16	22.623	14601	1230	0.101
17	24.016	1529	195	0.011
Total		14387467	1686029	100.000