

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E8888321F
 Time Processed :19:22:25
 Month-Day-Year Processed :06/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

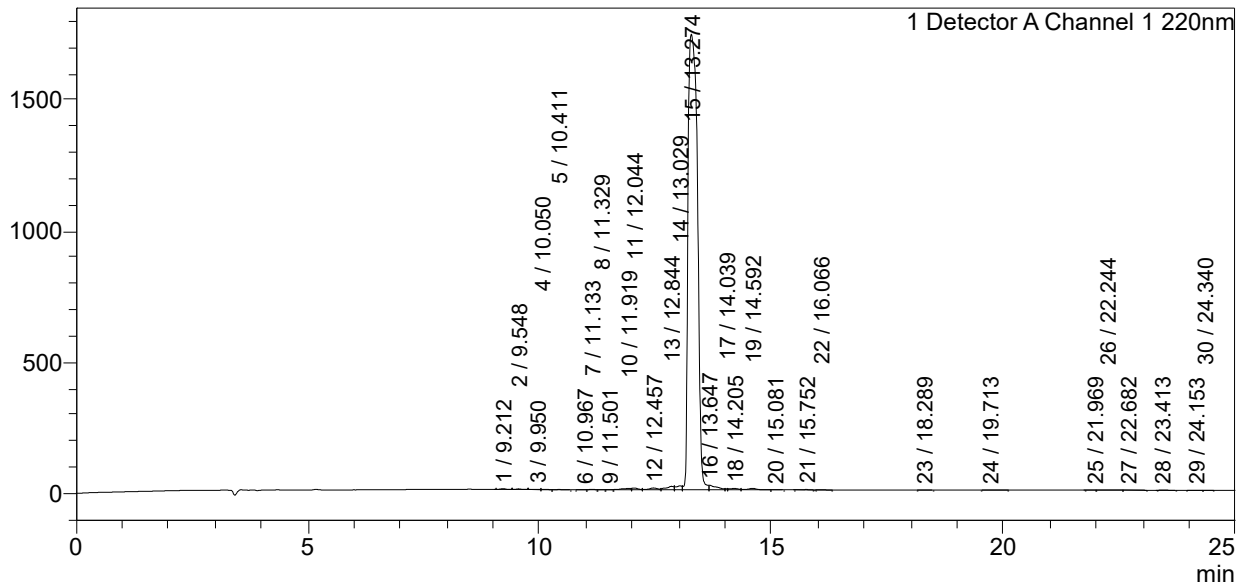

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.212	24259	3179	0.096
2	9.548	15688	2355	0.062
3	9.950	4340	443	0.017
4	10.050	3549	424	0.014
5	10.411	1844	189	0.007
6	10.967	1192	158	0.005
7	11.133	4535	658	0.018
8	11.329	2058	229	0.008
9	11.501	1653	255	0.007
10	11.919	60666	5055	0.240
11	12.044	57206	6226	0.227
12	12.457	76025	6433	0.301
13	12.844	164296	12603	0.651
14	13.029	120780	14843	0.479
15	13.274	24299352	1737231	96.287

Peak#	Ret. Time	Area	Height	Area%
16	13.647	209535	17246	0.830
17	14.039	17483	3541	0.069
18	14.205	54322	4327	0.215
19	14.592	59498	4932	0.236
20	15.081	1969	218	0.008
21	15.752	12679	1287	0.050
22	16.066	6083	744	0.024
23	18.289	1452	215	0.006
24	19.713	4198	283	0.017
25	21.969	1578	198	0.006
26	22.244	16302	654	0.065
27	22.682	7989	806	0.032
28	23.413	2761	232	0.011
29	24.153	1861	159	0.007
30	24.340	1099	151	0.004
Total		25236251	1825275	100.000