

Sample Name : CGRP (8-37), human
 Cat. No. : RP11089
 Lot. No. : PE0041812
 Time Processed : 13:43:08
 Month-Day-Year Processed : 12/13/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

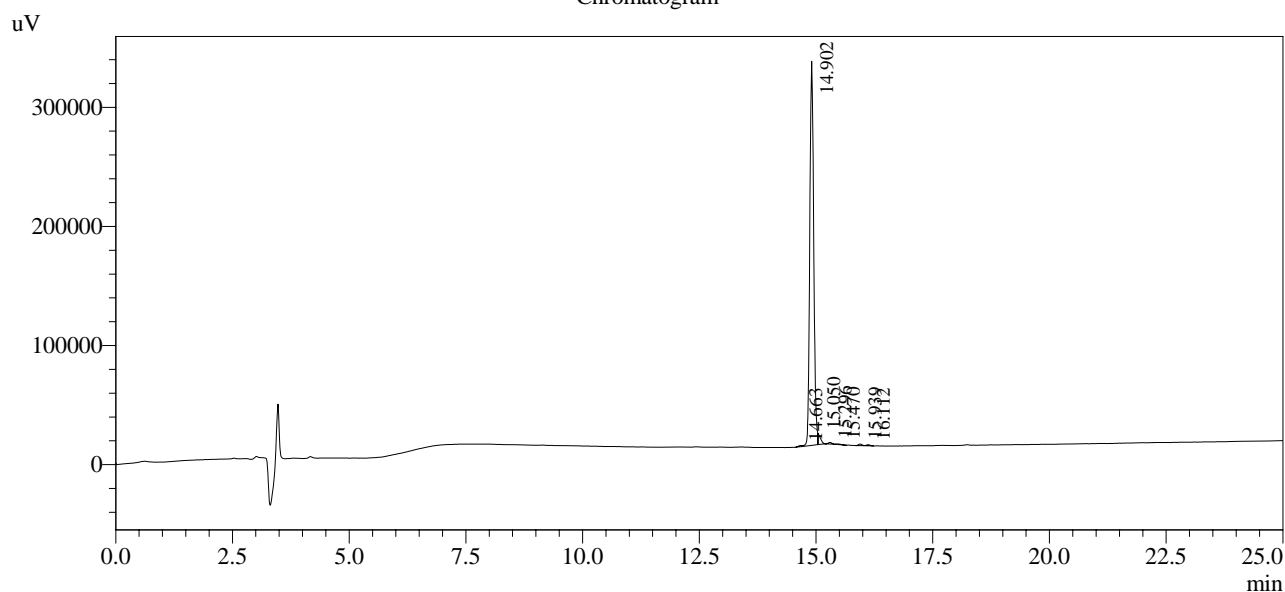

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.663	5483	1018	0.282
2	14.902	1887095	322540	96.892
3	15.050	32403	8709	1.664
4	15.296	7419	1313	0.381
5	15.470	3043	453	0.156
6	15.939	7151	1312	0.367
7	16.112	5032	951	0.258
Total		1947626	336297	100.000