

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017 Lot. No. :PE2501803

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	10	
40.00	Pumps	Pump A B.Conc	10	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

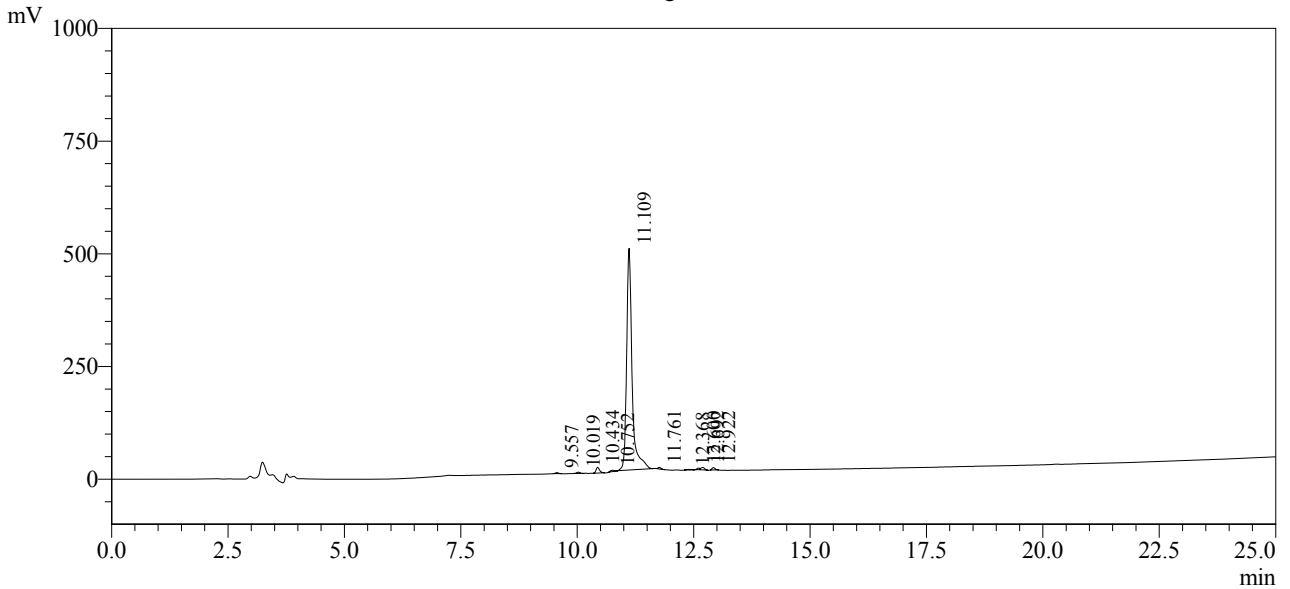

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.557	10438	2206	0.248
2	10.019	14035	2795	0.333
3	10.434	66068	12823	1.567
4	10.752	16876	2860	0.400
5	11.109	4011554	491961	95.161
6	11.761	16629	3507	0.394
7	12.368	11265	1473	0.267
8	12.600	16268	3640	0.386
9	12.692	28428	5499	0.674
10	12.922	24001	5017	0.569
Total		4215563	531780	100.000