

Sample Name :Transportan
 Cat No. :RP20512
 Lot No. :E4942019I
 Time Processed :8:46:53 AM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

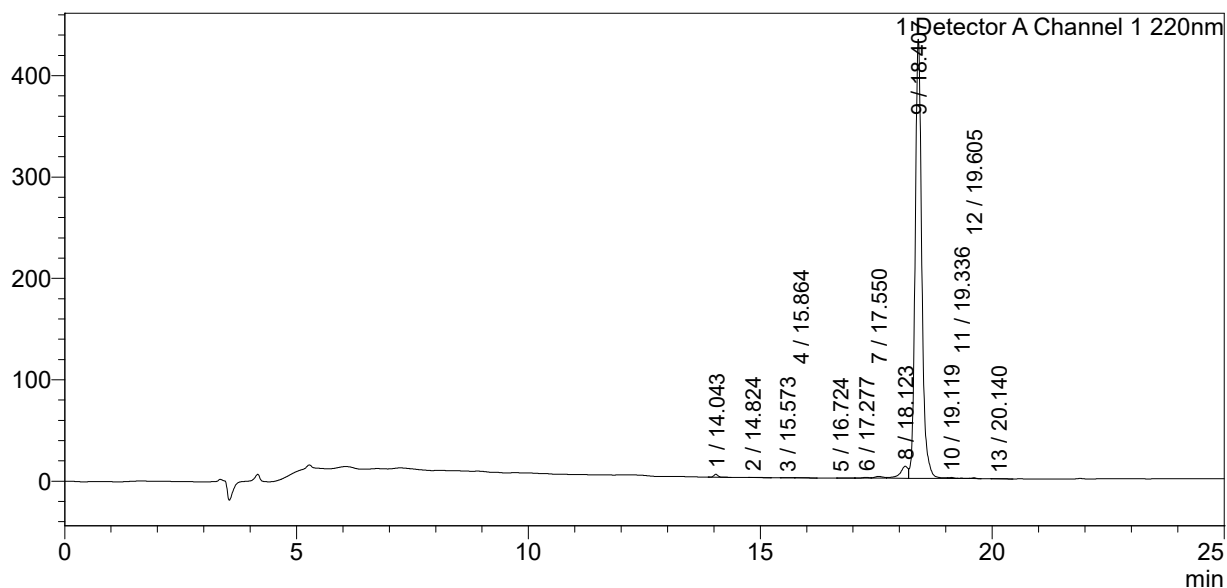

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.043	19158	2958	0.426
2	14.824	2576	163	0.057
3	15.573	1312	190	0.029
4	15.864	1907	158	0.042
5	16.724	1448	135	0.032
6	17.277	8065	707	0.180
7	17.550	22937	1772	0.511
8	18.123	140447	11887	3.127
9	18.407	4283651	433226	95.362
10	19.119	2874	540	0.064
11	19.336	1297	147	0.029
12	19.605	4487	790	0.100
13	20.140	1839	182	0.041
Total		4491999	452857	100.000