

Sample Name :Bradykinin
 Cat. No. : RP11129
 Lot. No. : E9408121D
 Time Processed :3:09:25
 Month-Day-Year Processed :05/06/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 5 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 27.00 | Pumps | B.Conc | 95 |
| 27.01 | Pumps | B.Conc | 5 |
| 35.00 | Pumps | B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0310

<Chromatogram>

mV

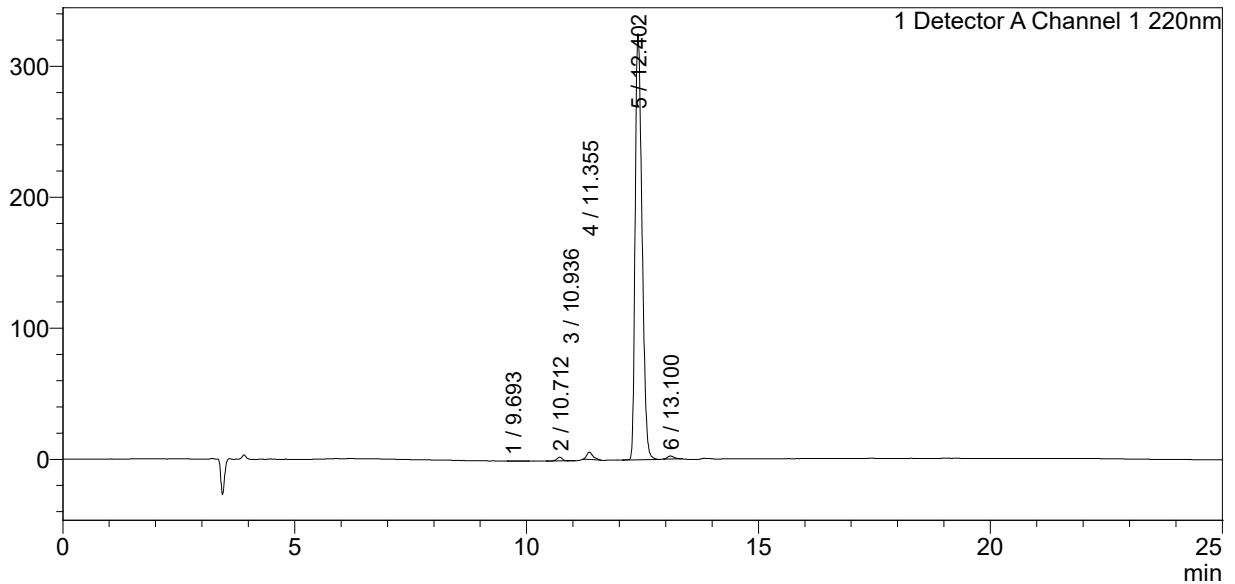

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 9.693 | 1562 | 118 | 0.045 |
| 2 | 10.712 | 24314 | 2918 | 0.705 |
| 3 | 10.936 | 604 | 111 | 0.017 |
| 4 | 11.355 | 50684 | 5489 | 1.469 |
| 5 | 12.402 | 3351120 | 325395 | 97.112 |
| 6 | 13.100 | 22506 | 2221 | 0.652 |
| Total | | 3450790 | 336253 | 100.000 |