

Sample Name :Protease-Activated Receptor-2, amide
 Cat No. : RP20334
 Lot No. : E5993120C
 Time Processed : 16:02:43
 Month-Day-Year Processed : 03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

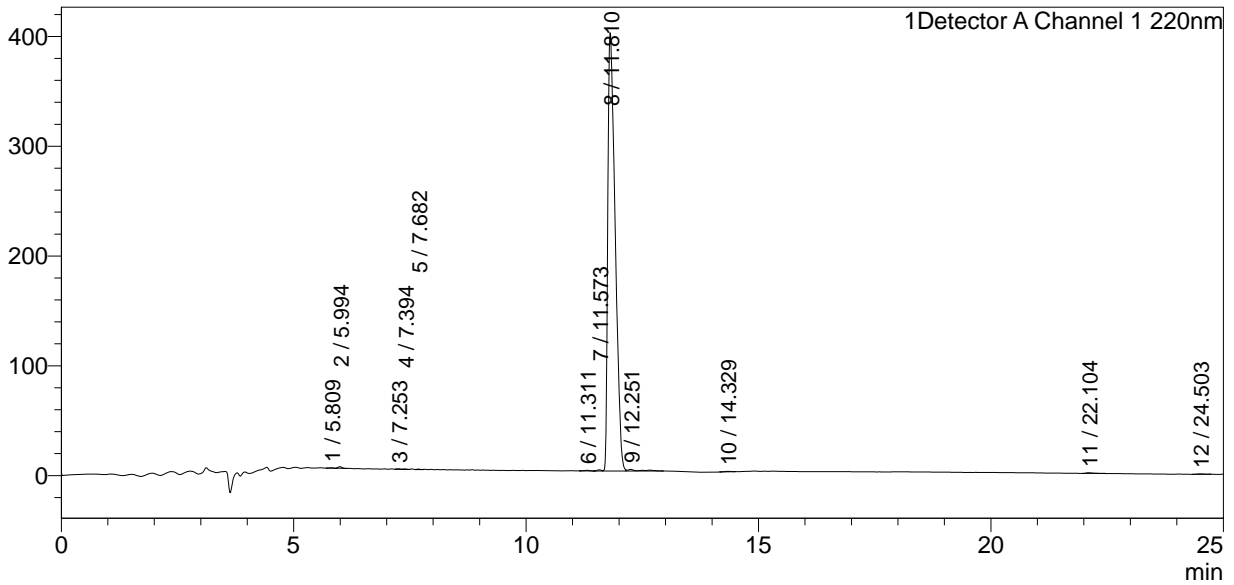

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.809	2394	367	0.054
2	5.994	8297	1463	0.187
3	7.253	2553	470	0.058
4	7.394	2102	462	0.047
5	7.682	1725	429	0.039
6	11.311	4412	606	0.099
7	11.573	6552	1056	0.148
8	11.810	4366349	397801	98.405
9	12.251	27995	1495	0.631
10	14.329	3554	438	0.080
11	22.104	7408	670	0.167
12	24.503	3765	402	0.085
Total		4437108	405660	100.000