

Sample Name :Angiotensin II (3-8), human
 Cat No. :RP11253
 Lot No. :E4725719I
 Time Processed :10:21:39
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

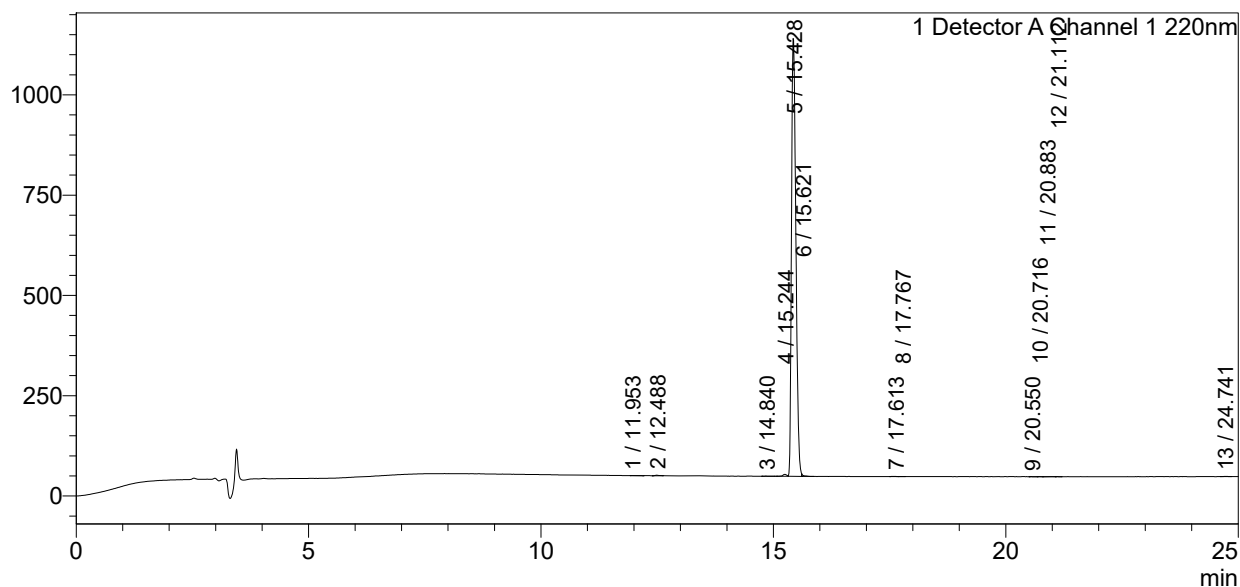

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.953	2095	205	0.029
2	12.488	7034	1380	0.097
3	14.840	2733	301	0.038
4	15.244	28225	5025	0.390
5	15.428	7169433	1091318	99.058
6	15.621	13931	4623	0.192
7	17.613	2917	418	0.040
8	17.767	1156	182	0.016
9	20.550	1357	213	0.019
10	20.716	1064	324	0.015
11	20.883	3031	219	0.042
12	21.112	1059	274	0.015
13	24.741	3552	485	0.049
Total		7237586	1104968	100.000