

Sample Name :YRGDS Fibronectin Fragment  
 Cat No.: RP20476  
 Lot No.: PE9361901  
 Time Processed:20:17:13  
 Month-Day-Year Processed:01/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

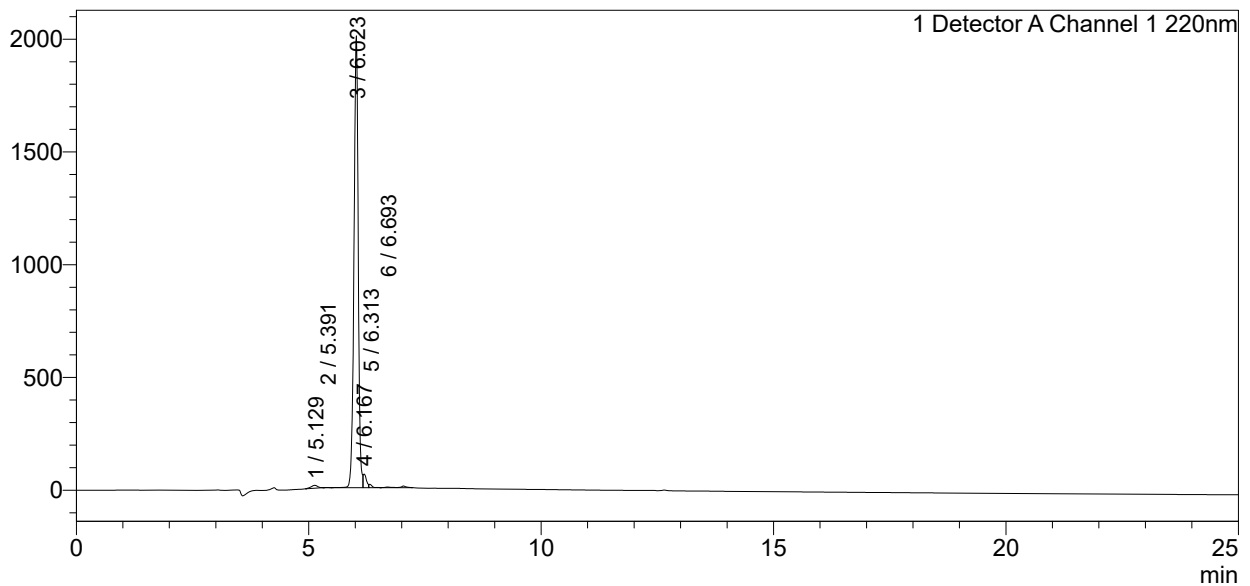

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.129	123821	12571	0.929
2	5.391	2253	361	0.017
3	6.023	12755675	2003134	95.733
4	6.167	289839	56396	2.175
5	6.313	64686	14719	0.485
6	6.693	87972	2885	0.660
Total		13324247	2090066	100.000