

Sample Name: Fibronectin CS1 Peptide  
 Cat No. : RP10838  
 Lot No. : E1435420G  
 Time Processed: 8:34:52 AM  
 Month-Day-Year Processed :08/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

<Chromatogram>

mV

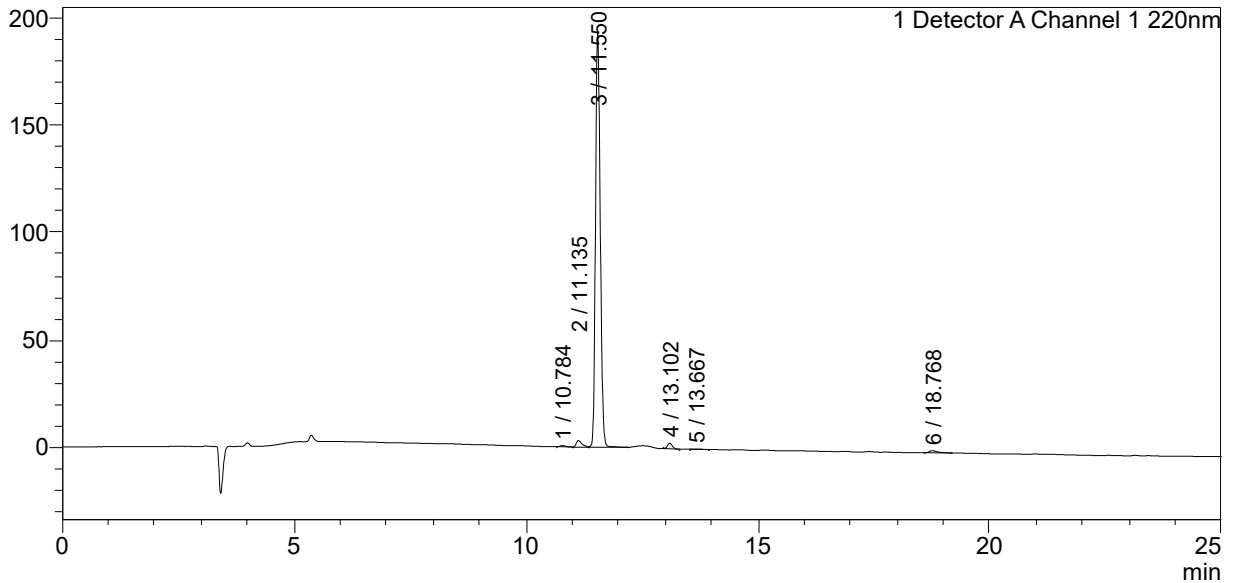

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.784	4957	591	0.343
2	11.135	26550	3115	1.838
3	11.550	1379410	193633	95.471
4	13.102	19151	2643	1.325
5	13.667	1645	115	0.114
6	18.768	13140	1033	0.909
Total		1444854	201130	100.000