

Sample Name : CLIP (86-100)
 Cat. No. : RP20279
 Lot. No. : PE1391707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


| Time | Unit | Command | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01 | Pumps | Pump A B.Conc | 5 | |
| 25.00 | Pumps | Pump A B.Conc | 65 | |
| 25.01 | Pumps | Pump A B.Conc | 95 | |
| 31.00 | Pumps | Pump A B.Conc | 95 | |
| 31.01 | Pumps | Pump A B.Conc | 5 | |
| 40.00 | Pumps | Pump A B.Conc | 5 | |
| 40.01 | Controller | Stop | | |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

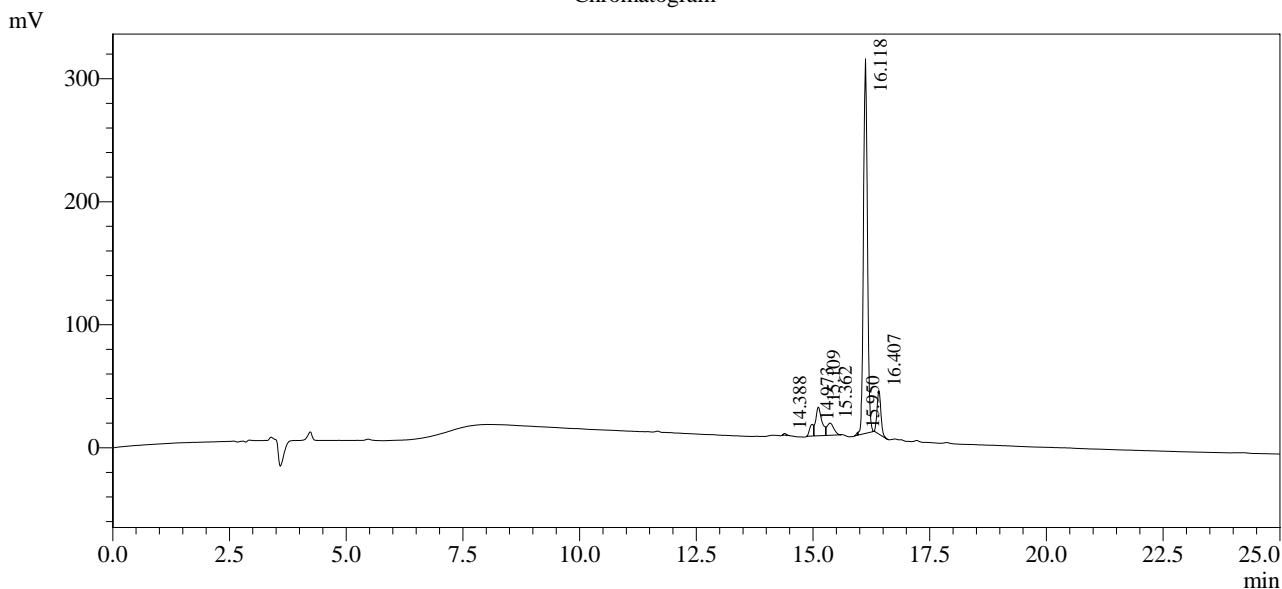

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 14.388 | 5956 | 1402 | 0.250 |
| 2 | 14.973 | 57271 | 9524 | 2.402 |
| 3 | 15.109 | 214539 | 23292 | 8.999 |
| 4 | 15.362 | 98174 | 9919 | 4.118 |
| 5 | 15.950 | 5140 | 2114 | 0.216 |
| 6 | 16.118 | 1802854 | 304537 | 75.626 |
| 7 | 16.407 | 199975 | 34882 | 8.389 |
| Total | | 2383909 | 385670 | 100.000 |