

Sample Name : Biotin-TAT (47-57)  
 Cat No. : RP20408  
 Lot No. : E7135721C  
 Time Processed : 23:39:12  
 Month-Day-Year Processed : 03/30/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : ZJ20010140

<Chromatogram>

mV

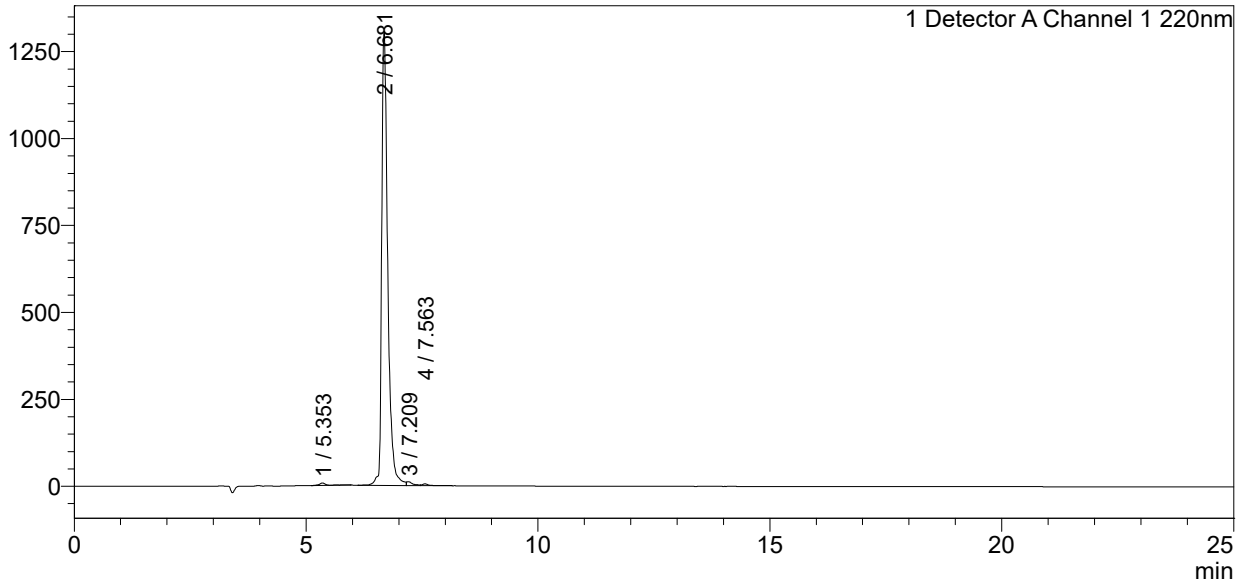

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.353	58060	6978	0.479
2	6.681	11907352	1305439	98.224
3	7.209	104887	11099	0.865
4	7.563	52386	5200	0.432
Total		12122685	1328715	100.000