

Sample Name :Parathyroid Hormone (PTH) (1-34), Human  
 Cat No :RP01001  
 Lot No :E2903720L  
 Time Processed :1:43:04 PM  
 Month-Day-Year Processed :01/03/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.10	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

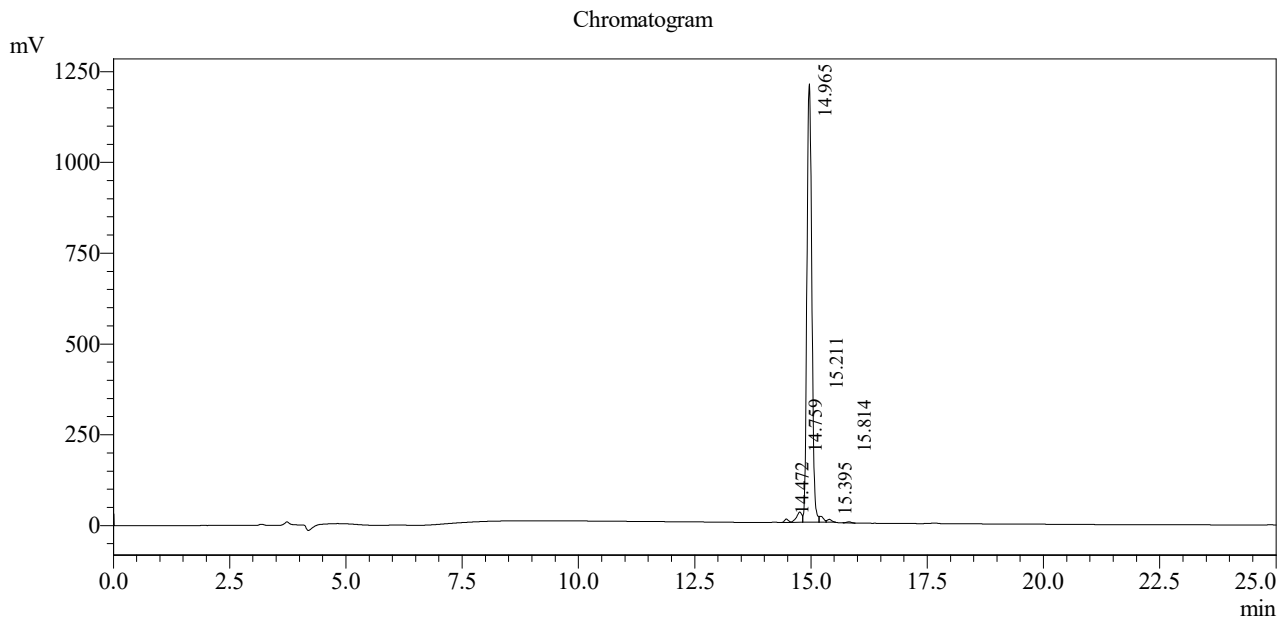

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.472	53188	9195	0.570
2	14.759	234777	28312	2.514
3	14.965	8877743	1207156	95.070
4	15.211	100409	16236	1.075
5	15.395	48831	7420	0.523
6	15.814	23117	3286	0.248
Total		9338064	1271606	100.000