

Sample Name :Hexa-His
 Cat No. : RP11737
 Lot No. : E9536521B
 Time Processed : 4:26:44 PM
 Month-Day-Year Processed : 03/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	10
25.00	Pumps	Pump A B.Conc	70
25.01	Pumps	Pump A B.Conc	95
30.00	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	10
40.00	Pumps	Pump A B.Conc	10
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

mV

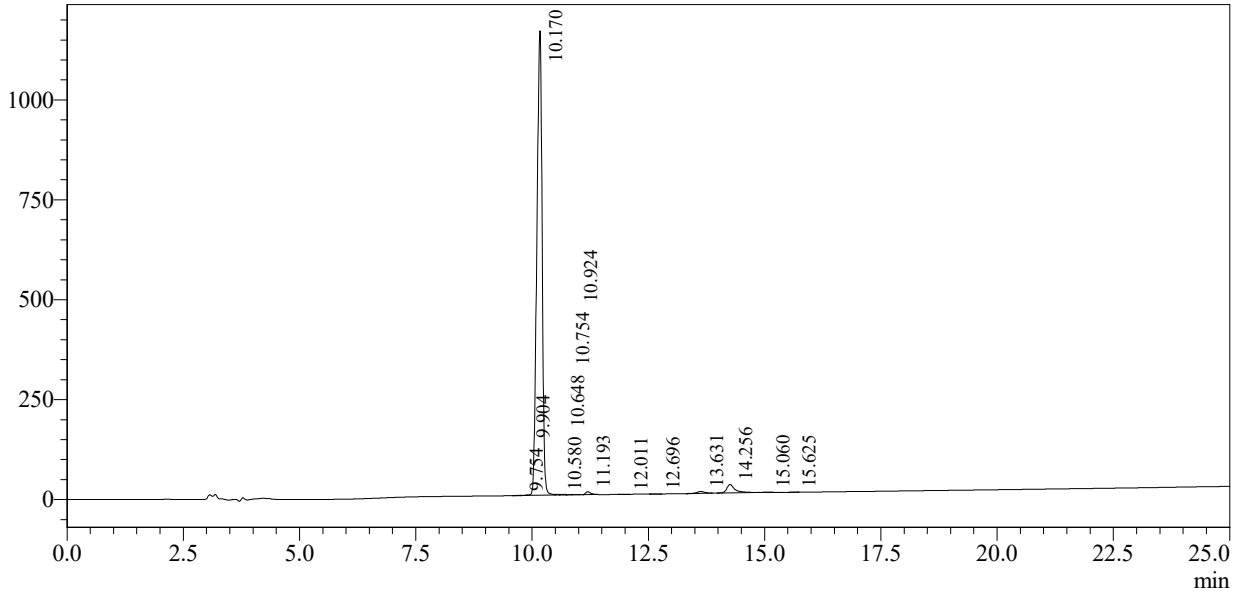

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.754	1620	84	0.017
2	9.904	4423	931	0.046
3	10.170	9153007	1161999	95.509
4	10.580	10222	1655	0.107
5	10.648	11648	1594	0.122
6	10.754	3665	809	0.038
7	10.924	3816	502	0.040
8	11.193	54148	7290	0.565
9	12.011	1966	168	0.021
10	12.696	974	120	0.010
11	13.631	54605	4727	0.570
12	14.256	264855	20824	2.764
13	15.060	17266	1264	0.180
14	15.625	1213	167	0.013
Total		9583429	1202136	100.000