

Sample Name: Influenza NP (147-155)
 Cat No: RP20260
 Lot No: E4438021E
 Time Processed : 17:30:42
 Month-Day-Year Processed : 05/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

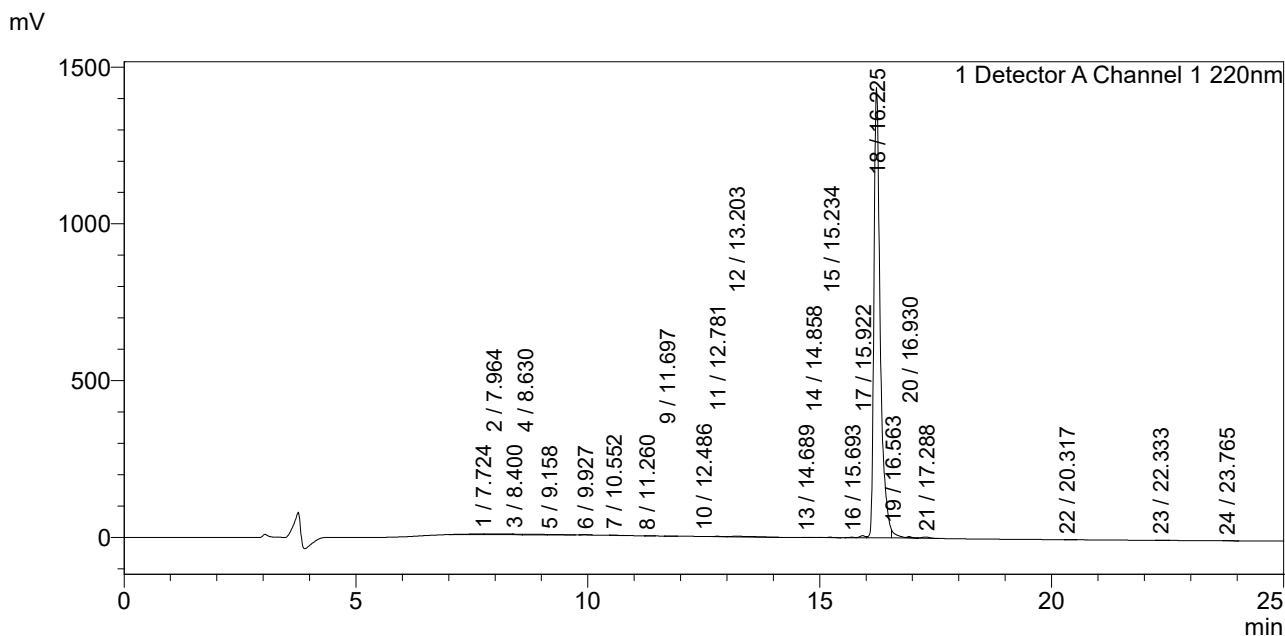

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.724	67833	2422	0.473
2	7.964	90500	2666	0.632
3	8.400	24717	2031	0.173
4	8.630	49338	1773	0.344
5	9.158	18374	1072	0.128
6	9.927	8903	1357	0.062
7	10.552	4835	353	0.034
8	11.260	1578	169	0.011
9	11.697	1015	165	0.007
10	12.486	1123	164	0.008
11	12.781	14898	766	0.104
12	13.203	78224	1974	0.546
13	14.689	1066	230	0.007
14	14.858	1455	164	0.010
15	15.234	14637	1285	0.102
16	15.693	13857	1560	0.097

Peak#	Ret. Time	Area	Height	Area%
17	15.922	55391	6770	0.387
18	16.225	13657259	1436213	95.318
19	16.563	161385	22820	1.126
20	16.930	18748	3295	0.131
21	17.288	39034	3669	0.272
22	20.317	1091	129	0.008
23	22.333	1016	135	0.007
24	23.765	1835	146	0.013
Total		14328111	1491327	100.000