


Mass Spectrum

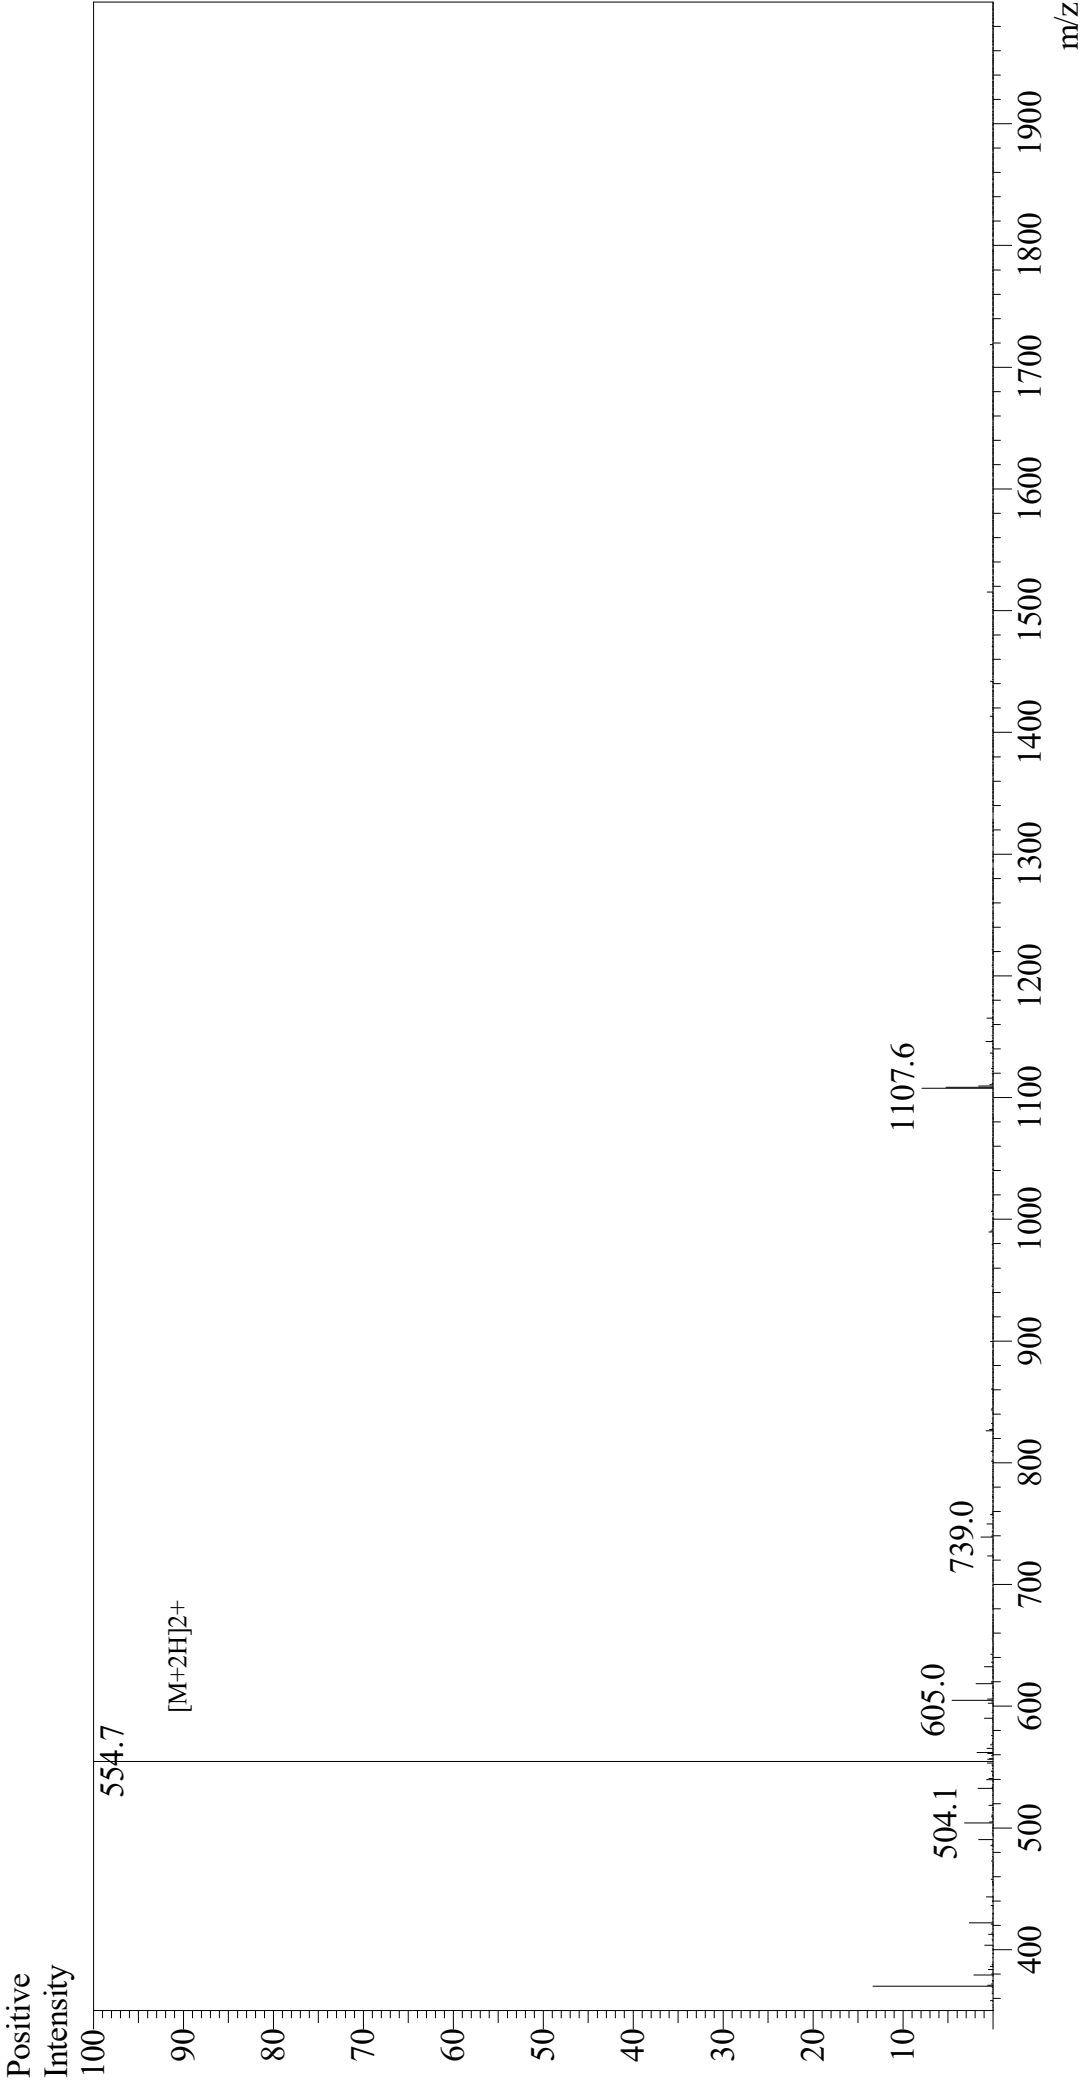

Sample Information
Month-Day Processed : 05/28/21
Time Processed : 7:27:13
Injection Volume : 0.4
Sample Name : Influenza NP (147-155)
SCat. No. : RP20260
Lot. No. : E4438021E
Theoretical MW : 1107.27
Observed MW : 1107.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH