

Sample Name : SV40 T-Ag-derived NLS peptide
 Cat. No. : RP20513
 Lot. No. : E4666619I
 Time Processed : 14:49:25
 Month-Day-Year Processed : 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

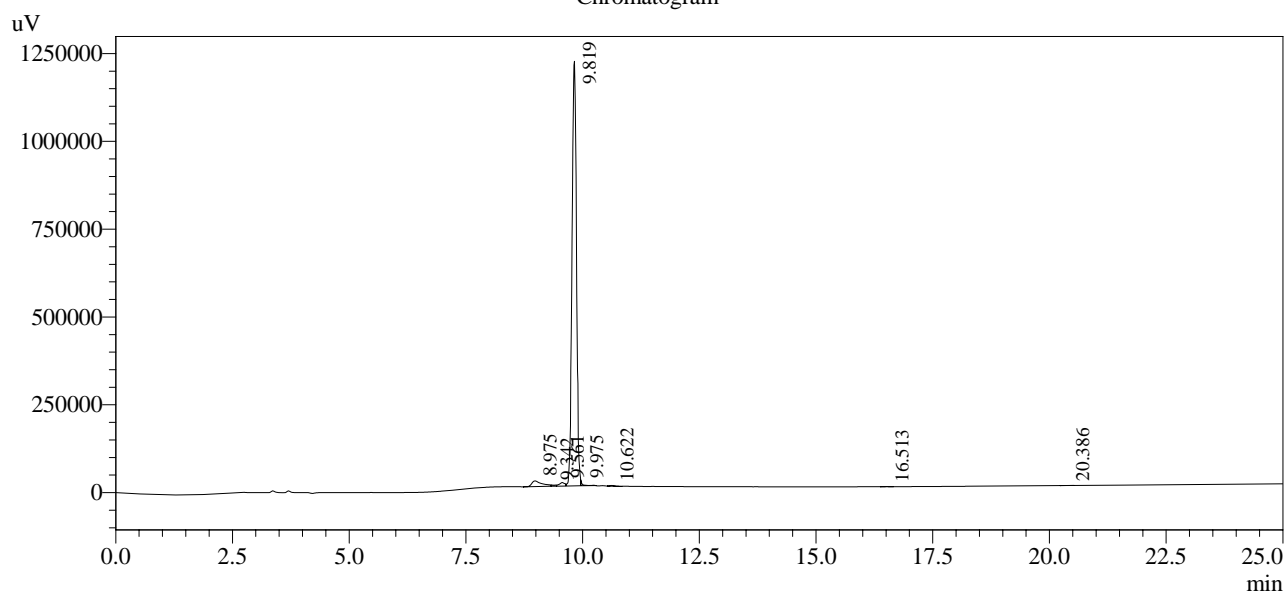

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.975	246466	16026	2.926
2	9.342	23537	3612	0.279
3	9.561	81970	9898	0.973
4	9.819	8024090	1203534	95.261
5	9.975	31806	10677	0.378
6	10.622	9834	1876	0.117
7	16.513	2101	363	0.025
8	20.386	3492	528	0.041
Total		8423296	1246514	100.000