

Sample Name : Gastrin-1, human
 Cat. No.: RP12740
 Lot. No. :E4895919I
 Time Processed :21:32:45
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	25	
25.00	Pumps	Pump A B.Conc	85	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	25	
40.00	Pumps	Pump A B.Conc	25	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

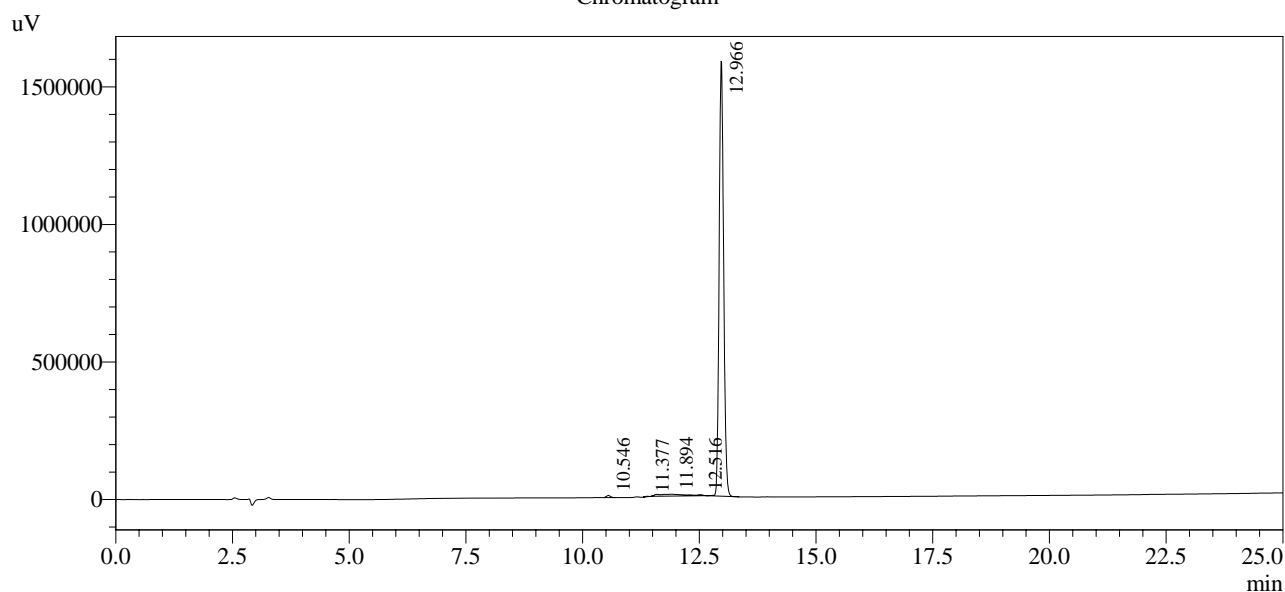

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.546	43951	7681	0.401
2	11.377	8580	1780	0.078
3	11.894	276697	7097	2.526
4	12.516	35305	4225	0.322
5	12.966	10589796	1581169	96.672
Total		10954328	1601953	100.000