

Sample Name: Angiotensin II, human  
 Cat No. :RP11257  
 Lot No. :E5929120K  
 Time Processed: 1:38:01 AM  
 Month-Day-Year Processed :11/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010325

<Chromatogram>

mV

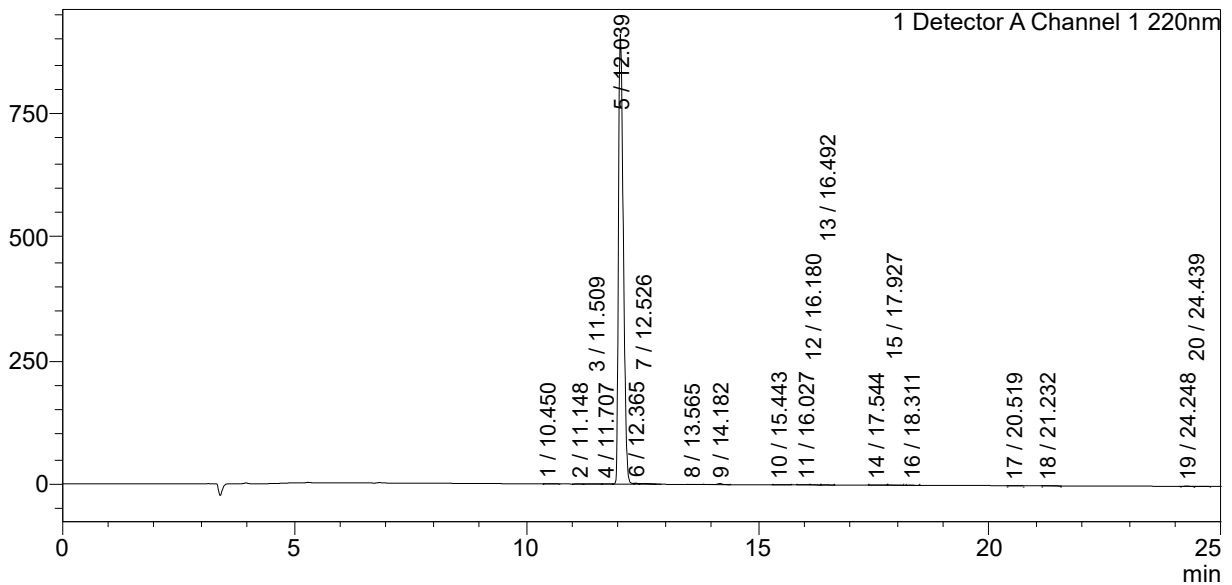

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.450	1142	129	0.017
2	11.148	1186	167	0.018
3	11.509	8132	770	0.122
4	11.707	6634	549	0.099
5	12.039	6618420	911730	99.095
6	12.365	2158	502	0.032
7	12.526	6256	604	0.094
8	13.565	1570	205	0.024
9	14.182	15950	2265	0.239
10	15.443	1694	122	0.025
11	16.027	1306	132	0.020
12	16.180	1474	214	0.022
13	16.492	1201	132	0.018
14	17.544	2042	168	0.031

Peak#	Ret. Time	Area	Height	Area%
15	17.927	1759	125	0.026
16	18.311	1078	132	0.016
17	20.519	1226	141	0.018
18	21.232	1519	167	0.023
19	24.248	2774	353	0.042
20	24.439	1363	156	0.020
Total		6678884	918764	100.000