

Sample Name : PGLa
 Cat. No. : RP17329
 Lot. No. : PE8631902
 Time Processed : 11:00:07
 Month-Day-Year Processed : 03/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

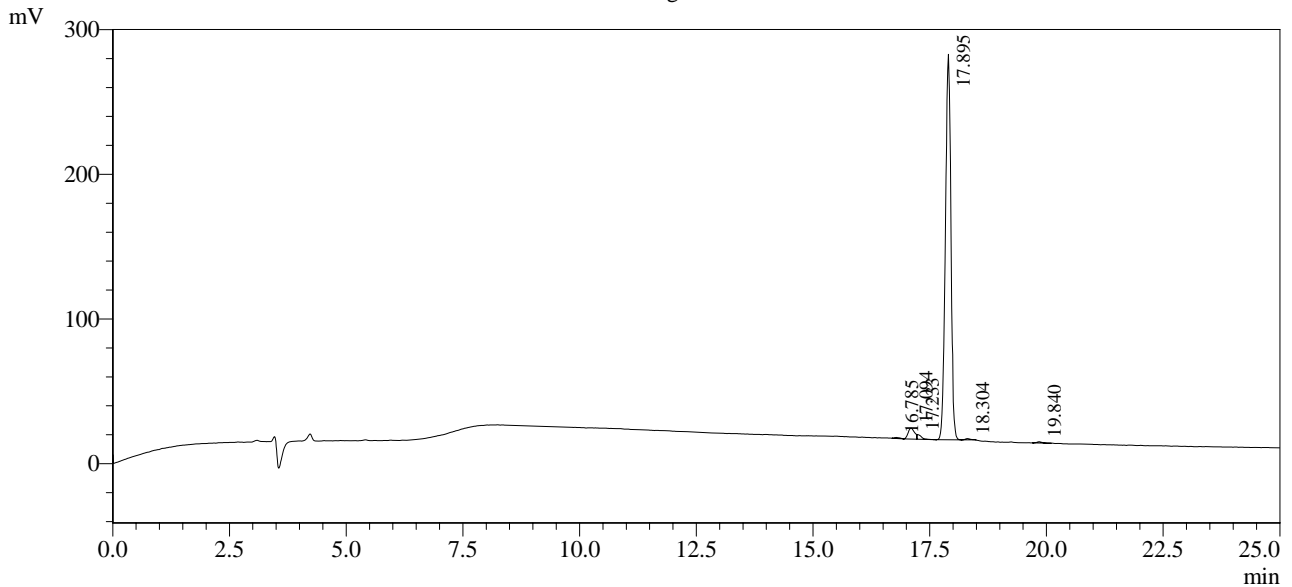

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.785	5491	656	0.238
2	17.094	73487	7601	3.182
3	17.233	21193	3236	0.918
4	17.895	2195285	266513	95.070
5	18.304	6772	858	0.293
6	19.840	6906	891	0.299
Total		2309134	279755	100.000