

Sample Name : VIP, human, ovine, porcine, rat  
 Cat No. : RP10085  
 Lot No. : E5106621A  
 Time Processed :10:23:52  
 Month-Dav-Year Processed :01/30/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
80.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

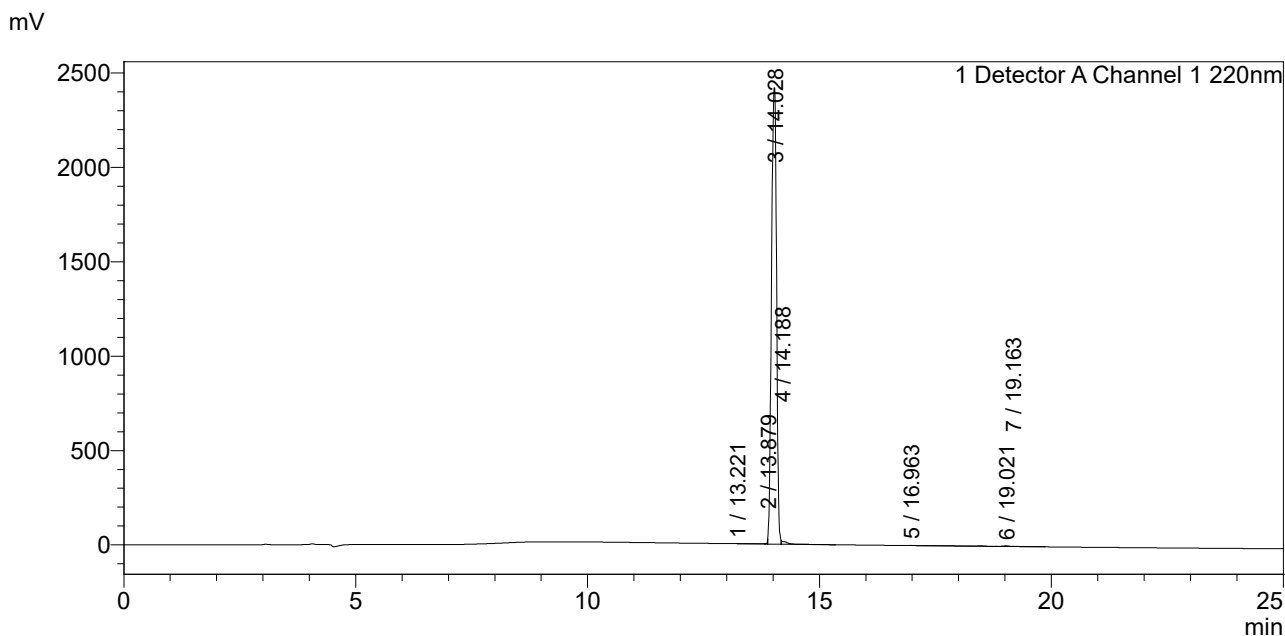

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.221	974	5	0.005
2	13.879	25050	13093	0.135
3	14.028	18281191	2418762	98.645
4	14.188	144644	16741	0.780
5	16.963	39413	14	0.213
6	19.021	34819	3982	0.188
7	19.163	6252	985	0.034
Total		18532343	2453582	100.000